
stomdevice

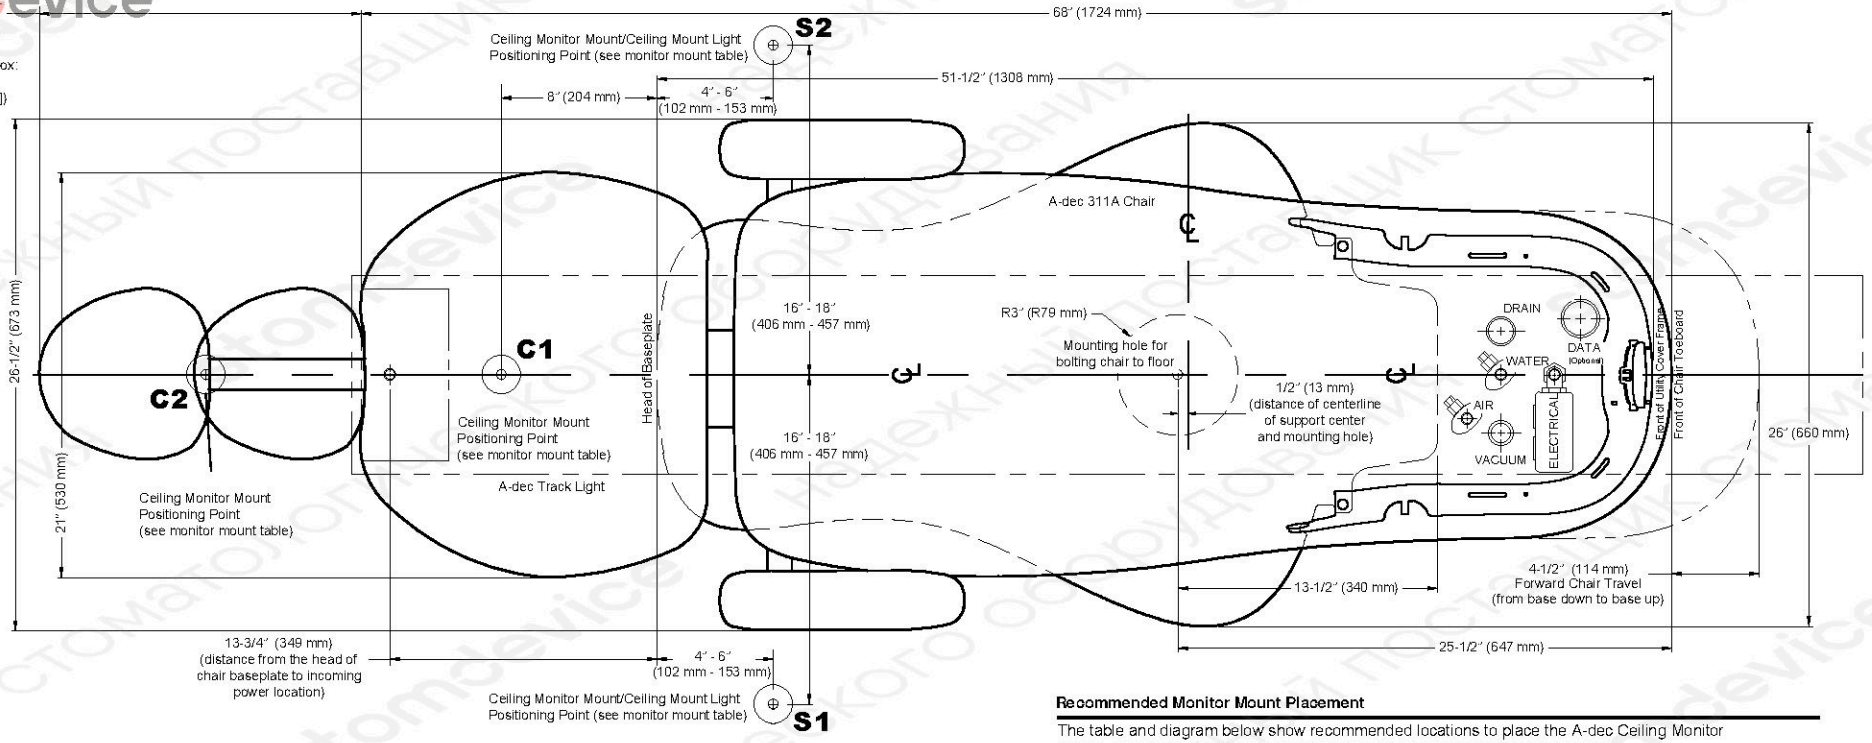

Recommended Monitor Mount Placement

The table and diagram below show recommended locations to place the A-dec Ceiling Monitor Mount. Primary recommendations minimize light and monitor arm interference.

IF THE SYSTEM HAS THIS TYPE OF LIGHT:	INSTALL THE MONITOR MOUNT HERE:	
	Primary Recommendation	Secondary Recommendation
Track-Mounted Ceiling Light	C2*	S1 or S2
Fixed-Mount Ceiling Light	C1	S1 or S2
Chair Mount Light	S1 or S2	C1
Preference-Mounted Light	S1 or S2	C1

* If installing at C2, position the monitor mount a minimum of 6-1/2" (165 mm) in front of the track light (towards 12 o'clock).

* NOTE: C2 postion restricts comfortable use of monitor to only supine patient position.


a-dec®
A-dec Headquarters
2601 Crestview Drive Newberg, Oregon 97132 USA
Tel: 1.800.547.1883 Within USA /Canada
Fax: 1.503.538.0276 Within USA /Canada
Tel: 1.503.538.7478 Outside USA /Canada
www.a-dec.com

A-dec 311A Dental Chair with Integrated Floor Box

Copyright 2021 A-dec Inc.
All rights reserved

86.0912.01 Rev E


A-dec 311 Plumbing Elevations

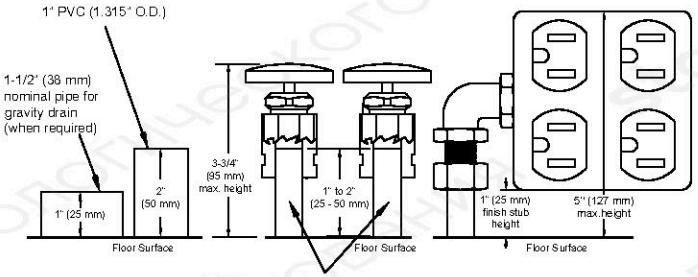

1/2" (13 mm) nominal pipe compression fitting with right-angle manual shutoff valves with 3/8" compression outlet for air and water (supplied by contractor)

PLEASE NOTE: **This drawing is for reference purposes ONLY. It is NOT TO SCALE.**

A-dec Track Light

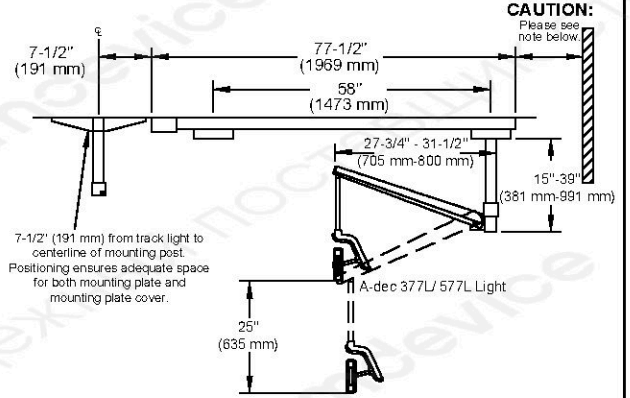

NOTE: If the track opposite the transformer is closer than 9-1/2" (241 mm) from a wall, the trolley and post assembly must be installed before the track is installed on the ceiling.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ