stomdevice

www.booool.com
Let's make things better

BaoLai Medical
Join us

X1 Device Instruction Manual

Please read the instruction manual carefully before operating


1 Symbol instruction

	Trademark
	Caution,consult accompanying documents
	Air outlet
5V	5VDC input


2 The conditions of working environment

Environmental temperature	+10℃ ~+40℃
Environmental humidity	0 ~80%
Atmospheric pressure	700hPa ~1060hPa

3 Sketch map

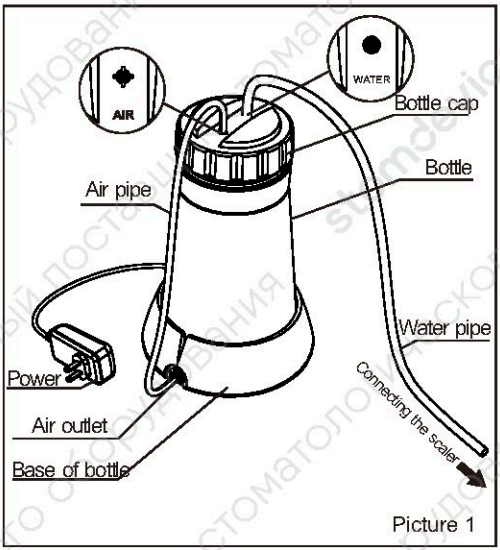

Picture 1

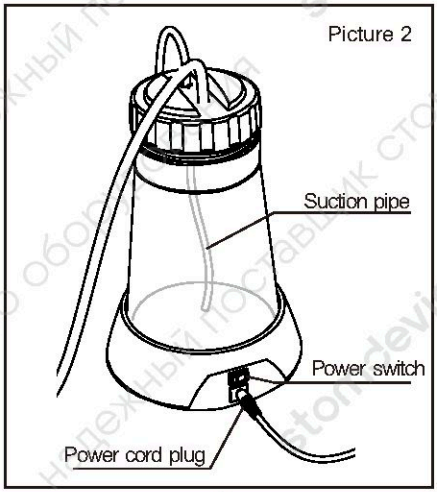

Picture 2

4 Usage

4.1 Open the packing,connect the device with scaler (Picture 1, Picture 2)
4.2 Inject water into the bottle,and screw tightly the bottle cap.
4.3 Connect the power socket.
4.4 Turn on the power switch to start the device.
4.5 Cut off the power source after finishing operation.

5 Cleaning and sterilization

5.1 Cleaning
Choose one of the following ways to clean bottle:
a) Cleaning with medical alcohol
b)Cleaning with special dental disinfection towel
5.2 Sterilization
Please use neutral sterilized liquid for cleaning the bottle and water pipe.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

6 Precautions ⚠

6.1 Please make sure all pipes are connected accurately and tightly before operating.
6.2 Please cut off the power source when inject or change water.
6.3 Do not exceed the maximum water volume of the bottle when inject water.
6.4 When the model is working, please don't pull the pipes forcibly in order to avoid damaging the air pipe and the water pipe.
6.5 Because there is air pressure in the bottle, please pull out the air pipe and the water pipe before open the bottle cap, and then inject water.
6.6 Please screw tightly the bottle cap after change water, and then turn on the power switch.
6.7 Please do not pull out the water pipe after completing pressurization in order to avoid water spraying from the bottle and cause secondary risk.
6.8 Please use the special configuration power supply of our company.
6.9 Repair of the equipment should be carried out by the manufacturer or by the authorized dealer.

7 Maintenance

7.1 Troubleshooting and notes

Fault	Possible cause	Solutions
There is no water flowing out after starting the device.	Air pressurization doesn't complete.	Please wait for one minute.
	Water pipe and air pipe connect incorrectly.	Refer to Picture 1.
	The bottle cap isn't screwed tightly.	Please screw tightly the bottle cap.
	The suction pipe isn't connected or it isn't connected tightly.	Please reconnect the suction pipe.
Pump doesn't work.	Don't connect the power or the power switch is off.	Please connect the power or turn on the power switch.
	Using the wrong power supply.	Please check whether you have used the special configuration power supply of our company.
Pump keeps working.	There is air leakage at the air pipe junction.	Please reconnect the air pipe.

If the problem still can't be solved, please contact with local dealer or manufacturer.

8 Storage and transportation

8.1 Environmental conditions of storage and transportation:
a) Relative humidity: 0 to 80%
b) Atmospheric pressure: 50kPa to 106kPa
c) Environmental temperature: -10℃ to +50℃
8.2 Prevent excessive shock and vibration in transportation, be sure to handle with care and avoid inversion.
8.3 Don't mix with dangerous goods during transportation.
8.4 Avoid the sun, rain or snow during transportation.
8.5 The equipment should be handled carefully and lightly. Be sure that it's far from the vibration, and install or store in a cool, dry and ventilated place.
8.6 Don't store the machine with the articles that are combustible, poisonous, caustic and explosive.

9 After-service

9.1 We offer 12 months free repair to the equipment based on warranty card from the date when it is sold to the end user.
9.2 The repair of the equipment should be carried out by our professional technician, irretrievable damage caused by the nonprofessional technician, and damage accidentally or deliberately caused by operators, are out of the range of warranty.

10 Environmental protections

10.1 You can deal with it based on the local law.
10.2 We reserve the right to change the design of the equipment, product technique, accessories, instruction manual and the content of original packing at any time without notice. If there are some differences between picture and real equipment, take the real equipment as the norm.

NANNING BAOLAI MEDICAL INSTRUMENT CO., LTD
Address: 7th Floor , General Building, Hetai Sci. &Tech. Park,No.9 Gaoxin 4th RD., Nanning,Guangxi, 530007, China
Service Number:0086-771-3815998 **E-mail:Info@booool.com**
Fax Number:0086-771-3217863 **Web:www.booool.com**
PA-X1-M-E-1 A2

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ