stomdevice

BESTMAN

JSO '
13435.

CE

ISO
aoo-j



BESTMAN

BV-520P

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ














2.4” TFT

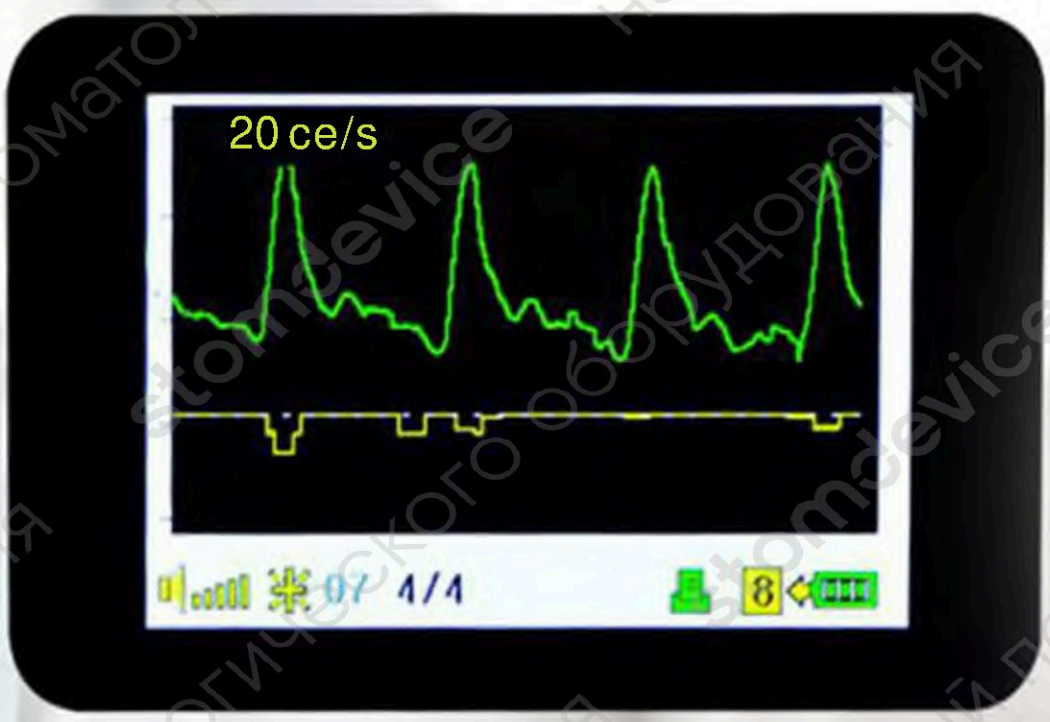


- 320 x 240 TFT display
- bidirection Real-time display of blood flow waveform and datadetect blood flow speed and frequency

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

BV-520P

Host built-in memory to store waveform and dataHost built-in memory to store waveform and data

Host built-in memory to store waveform and data

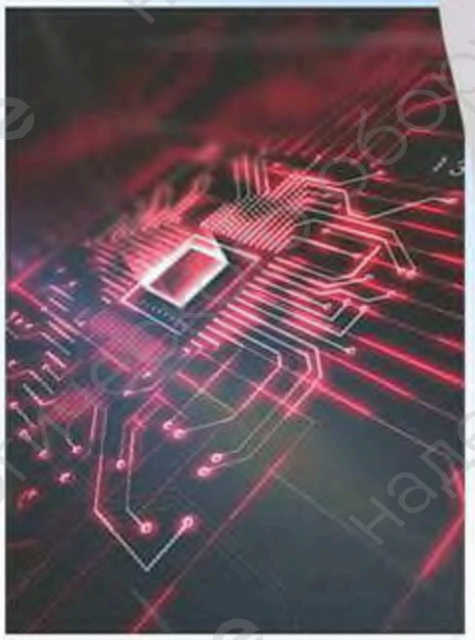







Even family members
You can also use it
Direct printing their own
checks, that it allows the
doctor to view the
spectrum
So you do not worry
about queuing rare
problem

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

Scope



Andrology



Plastic surgery



Surgery





Burn center



Built-in data interface, host can be used alone, or comply use with the computer.

Operating modes: continuous operation	Speed range: not narrower than 40cm / s - 200cm/ s
Band: The host 200 ± BO— 6000 ± 1000Hz	velocity error < 20% (relative error)
Probe: 350 ± 80 ~ 2500 ± 500Hz	System gain:> 100dB
External Output: Speaker	Audio bandwidth: 0.2 KHz ~ 7.0 KHz
Transmit waveform : sine	Display: 320x240 dot TFT
Ultrasonic frequency: 8.0MHz ± 10%	Total power consumption: <50W
Average sound intensity ultrasonic power < 50mW / cm2	Continuous working time: >8 hours



SHENZHEN BESTMAN INSTRUMENT CO.,LTD
www.szbestman.cn
Add: 8/F,YIFang Bldg,No.315 Shuangming Ave.Dongzhou Community, Guangming St..Guangming Dist., Shenzhen, Guangdong,518107, China
Tel: +86-755-26411423
Fax: +86-755-26495167

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ