stomdevice

Carestream DENTAL



CS 8100 3D Family

CS 8100 3D, CS 8100 3D Access, CS 8100SC 3D and CS 8100SC 3D Access

Safety, Regulatory and Technical Specifications User Guide

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Notice

The Regulatory Information and Technical Specifications User Guide for CS 8100 3D Family includes information on the safety instructions, regulatory information and the technical specifications of the devices. We recommend that you thoroughly familiarize yourself with this guide to make the most effective use of your system.

The CS 8100 3D Family comprises:

- CS 8100 3D: panoramic modality and dental volumetric reconstruction modality (3D focused teeth acquisition and 3D full upper and lower jaw acquisition).
- CS 8100 3D Access: panoramic modality and dental volumetric reconstruction modality (limited to 3D focused teeth acquisition). The system has the capability to expand the field of view to the 3D full upper and lower jaw acquisition with license upgrade.
- CS 8100SC 3D: panoramic modality, dental volumetric reconstruction modality (3D focused teeth acquisition and 3D full upper and lower jaw acquisition) and cephalometric modality.
- CS 8100SC 3D Access: panoramic modality, dental volumetric reconstruction modality (limited to 3D focused teeth application) and cephalometric modality (without the 26x24 Field of View (FoV)). The system has the capability to expand the field of view to the 3D full upper and lower jaw acquisition and to the cephalometric 26x24 FoV with licence upgrade.

This document refers to all models as CS 8100 3D Family unless otherwise specified.

The information contained in this guide may be subject to modification without notice, justification or notification to the persons concerned.

No part of this guide may be reproduced without the express permission of Carestream Health, Inc.

U.S. Federal law restricts this device to sale by or on the order of a dentist or physician.

This document is originally written in English.

Manual Name: CS 8100 3D Family Safety, Regulatory and Technical Specifications User Guide
Part Number: SM844
Revision Number: 08
Print date: 2016-09

CS 8100 3D Family comply with Directive 93/42/EEC relating to medical devices.

CE
0086

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Contents

1 Safety Information ..... - 4 -

Indications for Use ..... - 4 -
Conventions in this Guide ..... - 5 -
Note to the User ..... - 6 -
Warning and Safety Instructions ..... - 6 -
Hygiene and Disinfection ..... - 8 -
Marking and Labeling Symbols ..... - 13 -
Label Locations ..... - 14 -

2 Regulatory Information ..... - 17 -

General Regulatory Information ..... - 17 -
Compliance with International Regulations ..... - 22 -

3 Technical Specifications ..... - 23 -

Factory ..... - 23 -
Manufacturer ..... - 23 -
Model ..... - 23 -
CS 8100 3D Family Technical Specifications ..... - 23 -
Minimum Computer System Requirement ..... - 26 -
X-ray Dose Emission Information ..... - 27 -
Panoramic mode for CS 8100 3D and CS 8100 3D Access ..... - 27 -
3D mode for CS 8100 3D and CS 8100 3D Access ..... - 30 -
Panoramic mode for CS 8100SC 3D and CS 8100SC 3D Access ..... - 30 -
3D mode for CS 8100SC 3D and CS 8100SC 3D Access ..... - 30 -
Cephalometric mode for CS 8100SC 3D and CS 8100SC 3D Access ..... - 30 -
User Dose information ..... - 34 -
Stray radiation in Panoramic Mode ..... - 34 -
Stray radiation in 3D Mode ..... - 36 -
Imaging performance information ..... - 37 -
Panoramic and Cephalometric ..... - 37 -
3D ..... - 37 -
Controlling the Image Quality ..... - 37 -
CS 8100 3D Family Environmental Requirements ..... - 38 -
CS 8100 3D Family Electrical Specifications ..... - 39 -
X-ray Tube Assembly Technical Specifications ..... - 41 -

4 Contact Information ..... - 49 -

Manufacturer's Address ..... - 49 -
Factory ..... - 49 -
Authorized Representatives ..... - 49 -

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

1 Safety Information

Indications for Use

The CS 8100 3D Family is intended to produce complete or segmented tomographic digital panoramic images and three-dimensional digital X-ray images of the dento-maxillofacial area to be used at the direction of healthcare professionals as diagnostic support for pediatric and adult patients.
In addition, the CS 8100SC 3D and CS 8100SC 3D Access are also intended to produce cephalometric images. This includes imaging the hand and wrist to obtain carpus image for growth and maturity assessment.

The CS 8100 3D Family comprises:

- CS 8100 3D: panoramic modality and dental volumetric reconstruction modality (3D focused teeth acquisition and 3D full upper and lower jaw acquisition).
- CS 8100 3D Access: panoramic modality and dental volumetric reconstruction modality (limited to 3D focused teeth acquisition). The system has the capability to expand the field of view to the 3D full upper and lower jaw acquisition with license upgrade.
- CS 8100SC 3D: panoramic modality, dental volumetric reconstruction modality (3D focused teeth acquisition and 3D full upper and lower jaw acquisition) and cephalometric modality.
- CS 8100SC 3D Access: panoramic modality, dental volumetric reconstruction modality (limited to 3D focused teeth application) and cephalometric modality (without the 26x24 Field of View (FoV)). The system has the capability to expand the field of view to the 3D full upper and lower jaw acquisition and to the cephalometric 26x24 FoV with license upgrade.

This document refers to all models as CS 8100 3D Family unless otherwise specified.



WARNING: Do not use cone beam imaging for routine or screening examinations. Consider using other diagnostic tools. You must justify that the imaging method that you use to examine each patient demonstrates that the benefit outweighs the risks.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Conventions in this Guide

The following special messages emphasize information or indicate potential risk to personnel or equipment:



WARNING: Warns you to avoid injury to yourself or others by following the safety instructions precisely.



CAUTION: Alerts you to a condition that might cause serious damage.



Important: Alerts you to a condition that might cause problems.



Note: Emphasizes important information.



Tip: Provides extra information and hints.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Note to the User

WARNING: X-rays can be harmful and dangerous if not used properly. The instructions and warnings contained in this guide must be followed carefully.

As a manufacturer of radiology units that conform to stringent radiological protection standards in force throughout the world, we guarantee as low as reasonably achievable degree of protection against radiation hazards. Nonetheless, you are handling a radiology unit specially designed to emit X-ray doses in order to carry out a medical diagnosis.
The room in which your radiology unit is to be installed must comply with all official regulations applicable to protection against radiation. You must install your radiology unit in a room protected against X-ray emission.
Your local representative will assist you in the initial use of your radiology unit and will supply any relevant information you may require.
To use and operate the unit you must follow the instructions contained in this guide.

Warning and Safety Instructions

When operating CS 8100 3D Family, observe the following warning and safety instructions:



DANGER OF ELECTRIC SHOCK
This is an electrical unit. Do NOT expose it to water spray. Such action may cause an electric shock or a malfunction of the unit.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

WARNINGS

Unit

- **Read and understand this Safety Information before using the unit.**
- **You are responsible for the operation and maintenance of this unit. Only legally qualified persons can operate this unit. They MUST have training to use the radiological equipment. Do NOT open the cover of the unit. When necessary, have a trained authorized service technician carry out inspection and maintenance operations.**
- **Install this unit in an X-ray room that complies with current installation standards. From this location, you must be able to maintain visual or audio communication with the patient and be able to access the Acquisition interface module during exposure.**
- **This unit must be permanently connected to the ground with a fixed power supply cable. To avoid the risk of electric shock, this equipment must ONLY be connected to a mains supply with protective earth.**
- **Do NOT operate the unit if there is the threat of an earthquake. Following an earthquake, ensure that the unit is operating satisfactorily before using it again. Failure to observe this precaution may expose patients to hazards.**
- **X-ray equipment is hazardous to patients and the operator if you do not observe the exposure safety factors and operating instructions.**
- **Considering radiation safety of pediatric population, protocol for Acquisition on Pediatric patients must be followed. For more information on imaging pediatric patients more safely and effectively, refer to FDA Pediatric X-ray Imaging webpage:**
  http://www.fda.gov/radiation-emittingproducts/radiationemittingproductsandprocedures/medicalimaging/ucm298899.htm
- **Do NOT place objects within the field of operation of the unit.**
- **The patient should wear a protective lead-lined shoulder apron with a thyroid collar, unless other Radiation Protection Protocols apply locally.**
- **While adjusting the height of the unit, ensure that the patient is kept clear of the mechanism.**
- **When the unit is not in use, ensure that the ON/OFF switch is set to OFF (O).**
- **If the unit develops a fault, switch it to off (O), display an "Unserviceable" notice and contact a service technician.**
- **To dispose of the unit or its components, contact a service technician.**
- **Ask the patient to refrain from moving during the entire period of exposure.**
- **Ask the patient to remain still until the unit arm has stopped moving and the RESET movement has completed.**
- **Do NOT use this unit in conjunction with oxygen-rich environments. This unit is not intended for use with flammable anesthetics or flammable agents.**
- **Do NOT hang from the cephalostat**
- **It is not recommended to use accessories other than those specified in this document and sold by Carestream Health.**

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Computer

- **Do NOT place the computer and the peripheral equipment connected to it in the immediate vicinity of the patient in the unit. Leave at least 1.83m distance between the patient and the unit. The computer and the peripheral equipment must conform to the IEC 60950 standard.**
- **See your computer installation guide for details of the data processing system and screen. Leave a sufficient amount of clear space around the CPU to ensure that it is properly ventilated.**
- **To obtain maximum image quality and visual comfort, position the screen to avoid direct light reflections from internal or external lighting.**
- **Always use Microsoft Windows Update to make sure that the latest security patches are correctly installed.**

Hygiene and Disinfection

Cleaning the unit

To clean the unit, follow these steps:

1. Switch off the unit.

2. Remove all visible soil, if any, with disposable cloth or paper wipe.

Note: No disassembly shall be performed on the unit

3. Dampen (not soak) a lint-free cloth with soap and running water.

4. Thoroughly clean manually all accessible parts of the unit, including the temporal head clamps, with the dampened lint-free cloth.

5. Dry the unit with hygienic disposable cloth.

6. Dampen (not soak) a lint-free cloth with a low-level disinfectant that is U.S. Environmental Protection Agency (EPA)-registered or low-level disinfectant that is recognized by your Local Authority (for example, quaternary ammonium compounds and some phenolics). An EPA-registered hospital disinfectant or any other low-level disinfectant must have clear label claims for intended use.

7. Wipe thoroughly on all accessible parts of the unit with the dampened lint-free cloth. **You must follow the disinfectant's manufacturer instructions for use, especially with respect to contact time.**

8. Allow to dry in the open air for a minimum of 5 minutes.

9. Visually inspect the unit for signs of deterioration. If any damage is noted, do not use the unit and contact a service technician.

CAUTION
Avoid applying any cleaning liquid to the inside parts of the unit.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Cleaning and disinfecting the Accessories

Cleaning and disinfecting the accessories that have contact with the mucous membranes

CAUTION
You MUST cover the standard bite block and the bite block for edentulous patients with FDA-cleared or CE mark protective sheaths that are available from distributors to use them between each patient. We recommend that you cover the TMJ nose rest and the 3D bite blocks with FDA-cleared or CE Mark protective sheaths that are available from distributors to use them between each patient.

The following accessories must first be cleaned and then steam-sterilized between each patient use:

- TMJ nose rest
- Standard bite block
- Frankfort guide bite block for panoramic
- Bite block for edentulous patient
- 3D bite blocks

Note: It is recommended that the accessory be reprocessed as soon as reasonably practical following use.

Cleaning

To clean the accessories that have contact with the mucous membranes, follow these steps:

1. Remove and discard the protective sheath from the accessory.
2. Remove all visible soil by with disposable cloth or paper wipe.
3. Rinse at least 1 minute under running water to thoroughly clean the accessory from any excess soil.
4. Using a soft brush, apply medical enzyme detergent solutions (basically with a multi-enzymatic formula) to all surfaces of the accessory. **Detergent manufacturer's directions must be strictly adhered to.**
5. Rinse thoroughly under running water for at least 1 minute to remove detergent residue.
6. Dry the accessory with compressed air or hygiene disposable cloth.
7. Visually inspect the accessory for residual soil. If soil is visible, either repeat steps 2 to 5, or safely dispose of the accessory.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

Disinfecting with Steam Autoclave

To steam autoclave the accessory, once cleaning is complete, follow these steps:



CAUTION

You must use a medical autoclaving equipment cleared by the FDA in the USA or that is recognized by your Local Authority.
You must always follow the operating parameters recommended by the manufacturer of the autoclaving equipment.
Use FDA cleared or CE mark standard packaging material.

1. Wrap the cleaned accessory using a standard packaging material for autoclaving.
2. Steam autoclave at 132°C (270°F) for 4 minutes in the USA or depending on your local regulation you can steam autoclave at 134°C (273°F) for 18 minutes.
3. Visually inspect the accessory for signs of deterioration. If any damage is noted, do not use the accessory and contact your representative.
4. Once disinfected, the accessory can be used immediately or stored dry and dust-free in its sterilization wrapping under temperature specified in section “OS 8100 3D Family Environmental Requirements” of the present guide.

Cleaning and disinfecting Ear cones of CS 8100SC 3D and CS 8100SC 3D Access



CAUTION

Ear cones must be covered with a use FDA-cleared or CE mark protective sheaths that are available from distributors to use them between each patient. After use, remove and discard the protective sheath. You must clean and disinfect the ear cones between each patient use with an EPA-registered, or CE mark, intermediate-level disinfectant with label claims of tuberculocidal activity.

Cleaning

To clean the ear cones, follow these steps:

1. Remove and discard the protective sheath from the accessory.
2. Remove all visible soil with disposable cloth or paper wipe.
3. Dampen (not soak) a lint-free cloth with soap and running water.
4. Thoroughly clean manually the ear cones with the dampened lint-free cloth.
5. Rinse thoroughly with lint-free cloth with running water.
6. Dry the accessory with hygienic disposable cloth.
7. Visually inspect the accessory for residual soil. If soil is visible, either repeat steps 2 to 6, or safely dispose of the accessory.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Disinfecting

1. Use an intermediate-level disinfectant with tuberculocidal activity as identified above and as recommended by the manufacturer of the disinfectant.

2. Allow to dry in open air.

Cleaning and disinfecting the accessories and the components that have skin contact

The following accessories must first be cleaned and then disinfected between each patient use:

- Panoramic chin rest
- Sinus chin rest
- Temple support cone

The following component and accessory of the OS 81 OOSO 3D and CS 81 OOSC 3D Access must first be cleaned and then disinfected between each patient use:

- Nasion support
- Frankfort tool
- Carpus support (available only with Carpus exam option)

Note: It is recommended that the accessory be reprocessed as soon as reasonably practical following use.

Cleaning

To manually clean the accessories that have skin contact, follow these steps:

1. Remove all visible soil by with disposable cloth or paper wipe.

2. Rinse at least 1 minute under running water to thoroughly clean the accessory from any excess soil.

3. Using a soft brush, apply medical enzyme detergent solutions (basically with a multi-enzymatic formula) to all surfaces of the accessory. **Detergent manufacturer's directions must be strictly adhered to.**

4. Rinse thoroughly under running water for at least 1 minute to remove detergent residue.

5. Dry the accessory with compressed air or hygiene disposable cloth.

6. Visually inspect the accessory for residual soil. If soil is visible, either repeat steps 1 to 4, or safely dispose of the accessory.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Disinfecting

To disinfect the accessory, once the cleaning is complete, follow these steps:

1. Disinfect the accessory by using an EPA-registered hospital disinfectant for low-level activity or low-level disinfectant that is recognized by your Local Authority (for example, quaternary ammonium compounds and some phenolics). You must follow the disinfectant's manufacturer instructions for use, especially with respect to contact time.



CAUTION
If there is a visible contamination with blood, you must clean the accessory with an EPA-registered hospital disinfectant for intermediate-level disinfectant or intermediate-level disinfectant that is recognized by your Local Authority that has claim for activity against hepatitis B after cleaning. The disinfectant's manufacturer instructions for use must always be followed, especially with respect to contact time.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Marking and Labeling Symbols

	Type B device symbol complying with the IEC 60601-1 standard.
	In the European Union, this symbol indicates: Do NOT discard this product in a trash receptacle; use an appropriate recovery and recycling facility. Contact your local sales representative for additional information on the collection and recovery programs available for this product.
	WARNING Attention, consult Accompanying document
	IONIZING RADIATION symbol warn you about radiation dangers.
	The ON/OFF button.
	Refer to instruction manual/booklet
	Manufactured Date.
	Manufacturer's address.
	Earth protection (ground).


https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

Label Locations

CS 8100 3D and CS 8100 3D Access Labels

The following figure illustrates the label locations of the CS 8100 3D and CS 8100 3D Access.

Figure 1 CS 8100 3D and CS 8100 3D Access Label Locations

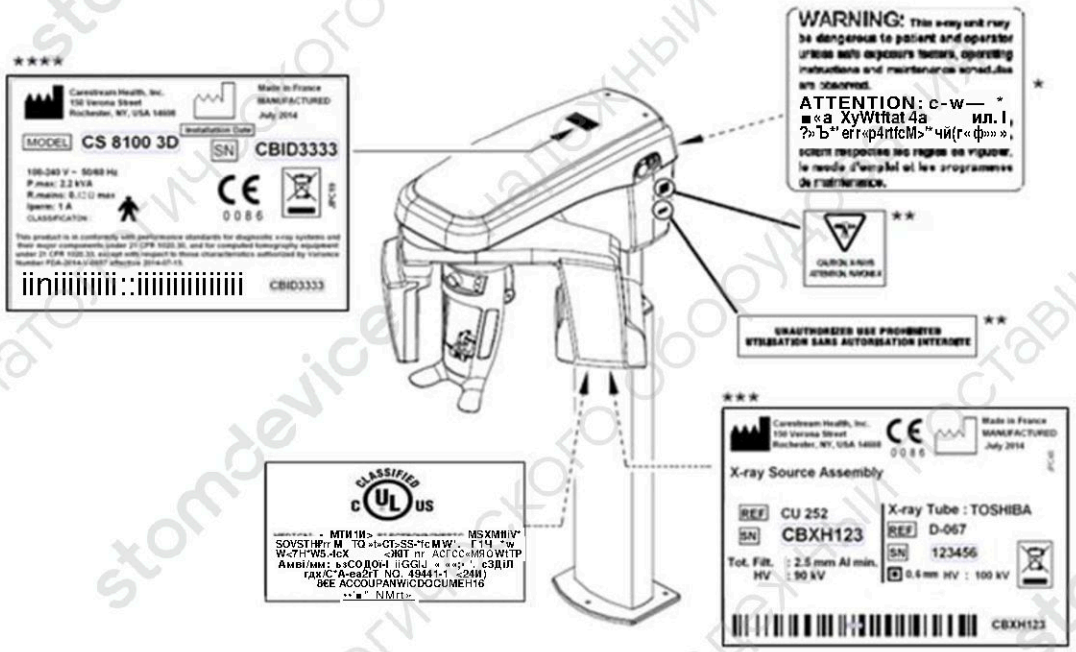

Important:

*** Only for USA: This warning appears in the Parameter pane of the Acquisition interface.**

**** Canada specific labels**

***** X-ray tube can be CEI OPX110**

****** Product label can be CS 8100 3D or CS 8100 3D Access**


https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

CS 8100SC 3D and CS 8100SC 3D Access Labels

The following figure illustrates the label locations of the CS 8100SC 3D and CS 8100SC 3D Access.

Figure 2 CS 8100SC 3D and CS 8100SC 3D Access Label Locations

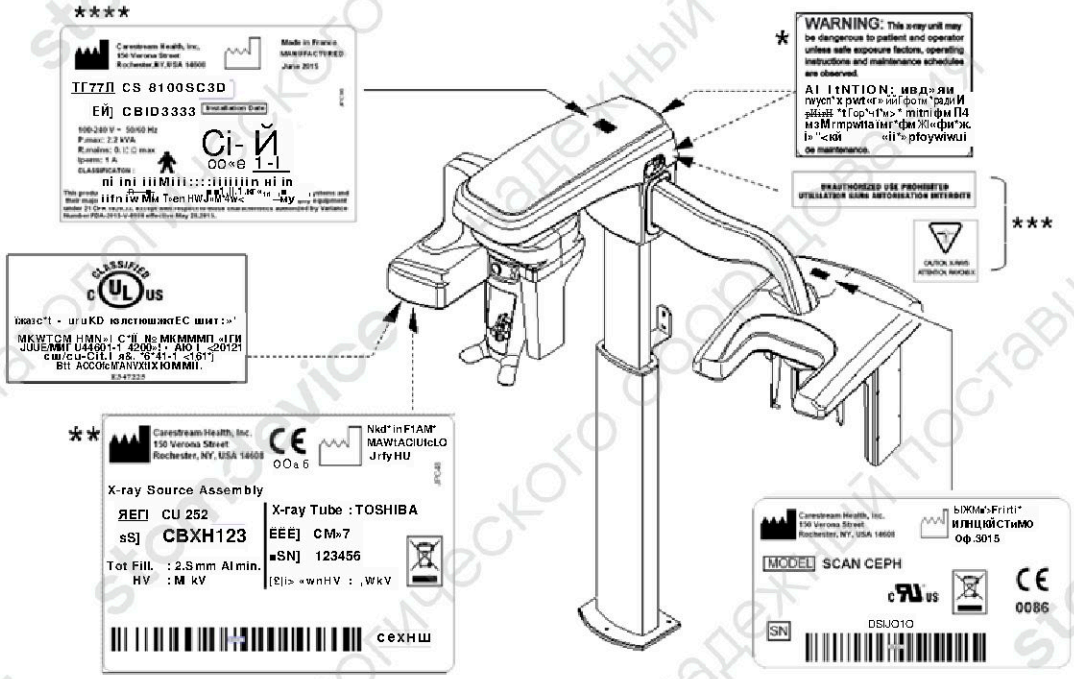

Important:

*** Only for USA: This warning appears in the Parameter pane of the Acquisition interface.**

**** X-ray tube can be CEI OPX110**

***** Canada specific labels**

****** Product label can be CS 8100SC 3D or CS 8100SC 3D Access**

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Table 1 Label Definition

Label	Definition
[MODEL]	Defines the unit's model
In Sts I37.Oл Date	Defines the date that the unit was installed
This product is in conformity with performance standards for diagnostic X-ray systems and their major components under 21 CFR 1020.30, and for computed tomography equipment under 21 CFR 1020.33, except with respect to those characteristics authorized by Variance Number FDA-2014-V-0657 effective 2014-07-15.	Defines the unit's compliance with the US FDA radiation standards Only applicable for CS 8100 3D
This product is in conformity with performance standards for diagnostic X-ray systems and their major components under 21 CFR 1020.30, and for computed tomography equipment under 21 CFR 1020.33, except with respect to those characteristics authorized by Variance Number FDA-2015-V-0980 effective 2015-05-28.	Defines the unit's compliance with the US FDA radiation standards Only applicable for CS 8100 3D Access

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

2 Regulatory Information

General Regulatory Information

Compliance with European and International Standards	
EN/IEC 60601-1	Medical Electrical Equipment - Part 1: General Requirements For Safety and essential performance.
EN/IEC 60601-1-2	Medical Electrical Equipment, Part 1-2: General requirements for basic Safety and essential performance - Collateral Standard: Electromagnetic Disturbances - Requirements and tests.
EN/IEC 60601-1-3	Medical Electrical Equipment, Part 1-3: General requirements for basic Safety and essential performance - Collateral Standard: Radiation protection in diagnostic X-ray equipment.
EN/IEC 60601-1-6	Medical Electrical Equipment, Part 1-6: General requirements for basic Safety and essential performance - Collateral Standard: Usability.
EN/IEC 62366	Medical devices - Application of usability engineering to medical device.
EN/IEC 62304	Medical device software – Software life cycle processes.
EN/IEC 60601-2-63	Medical Electrical Equipment - Part 2-63: Particular requirements for the basic safety and essential performance of dental extra-oral X-ray equipment.
EN 980	Symbols for use in the labeling of medical devices.
EN 1041	Information supplied by the manufacturer of medical devices.
ISO 10993-1	Biological evaluation of medical devices - Part 1: Evaluation and testing.
ISO 14971	Medical devices - Application of risk management to medical devices.
CAN/CSA C22.2 N° 60601-1	Medical Electrical Equipment - Part 1: General Requirements For Safety and essential performance.
ANSI/AAMI ES60601-1	Medical Electrical Equipment - Part 1: General Requirements For Safety and essential performance.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Classification in Accordance with EN/IEC 60601-1	
Type of protection against electric shock	Class 1 equipment
Degree of protection against electric shock	Type B
Protection against harmful ingress of water	Ordinary equipment
Operation mode	Continuous operation with intermittent loading
Flammable anesthetics	Not suitable for use in presence of flammable anesthetics or a mixture of flammable anesthetics with air or oxygen or nitrous oxide

Conformity with EN/IEC 60601-1-2
Group I, class B

CS 8100 3D Family is intended to be used in a professional healthcare facility environment.

Conformity with EN/IEC 60601-1-2
Electromagnetic Compatibility Precautions

- Medical electrical equipment requires special precautions regarding electromagnetic compatibility (EMC).
- CS 8100 3D Family must be installed and put into service according to the EMC information provided in this document.
- CS 8100 3D Family may interfere with other equipment even if that other equipment complies with CISPR emission requirements.
- Portable and Mobile RF communications equipment can affect medical electrical equipment.

CS 8100 3D Family System Components
Compliance to CS 8100 3D Family was achieved using the following cables: ▪ 1 main power supply cable (maximum length of 3 m) ▪ 1 Ethernet cable (maximum length of 10 m) ▪ 1 X-ray switch cable (maximum length of 10 m)

WARNINGS

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

- **Use limitation: the use of accessories, cables, or transducers other than those specified in the user's guide with the exception of cables, accessories or transducers sold by Carestream Health, Inc. as replacement parts of internal components may result in increased emissions or decreased immunity of the CS 8100 3D Family.**
- **Use limitation: the use of CS 8100 3D Family adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, the CS 8100 3D Family equipment and the other equipment should be observed to verify that they are operating normally.**
- **Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 1 m (39 in) to any part of the CS 8100 3D Family including cables specified by Carestream. Otherwise, it could result in degradation of the performance of the CS 8100 3D Family equipment.**

WARNING: The room in which your radiology unit is to be installed must comply with all official regulations applicable to protection against radiation.

Guidance and Manufacturer's Declaration - Electromagnetic Emissions (IEC 60601-1-2)		
The CS 8100 3D Family is intended for use in the electromagnetic environment specified below. The customer or the user of the CS 8100 3D Family should assure that it is used in such an environment.		
Emissions Test	Compliance	Electromagnetic Environment - Guidance
RF emissions CISPR 11	Group 1	The CS 8100 3D Family uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class B	The CS 8100 3D Family is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonic emissions IEC 61000-3-2	Class A	
Voltage fluctuations/ flicker emissions IEC 61000-3-3	Complies	

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Guidance and Manufacturer's Declaration - Electromagnetic Immunity			
The CS 8100 3D Family is intended for use in the electromagnetic environment specified below. The customer or the user of the CS 8100 3D Family should assure that it is used in such an environment.			
Immunity Test	**IEC 60601 Test Level**	**Compliance**	**Electromagnetic Environment - Guidance**
Electrostatic discharge (ESD) IEC 61000-4-2	±6 kV contact ±8 kV air	±8 kV contact ±15 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30 %.
Electrical fast transient/burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/output lines	±2 kV for power supply lines ±1 kV for input/output lines	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	±1 kV line(s) to line(s) ±2 kV line(s) to earth	±1 kV line(s) to line(s) ±2 kV line(s) to earth	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	<5 % UT (>95 % dip in UT) for 0.5 cycle 40 % UT (60 % dip in UT) for 5 cycles 70 % UT (30 % dip in UT) for 25 cycles <5 % UT (>95 % dip in UT) for 5 s	0 % UT for 0.5 cycle at 8 angles At 0°, 0 % UT for 1 cycle and 70 % UT for 25 cycles	Mains power quality should be that of a typical commercial or hospital environment. If the user of the CS 8100 3D Family requires continued operation during power mains interruptions, it is recommended that the CS 8100 3D Family be powered from an uninterruptible power supply or a battery.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	3 A/m	30 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment
NOTE: UT is the a.c. mains voltage prior to application of the test level.			

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Guidance and Manufacturer's Declaration - Electromagnetic Immunity (IEC 60601-1-2)

The CS 8100 3D Family is intended for use in the electromagnetic environment specified below. The customer or the user of the CS 8100 3D Family should assure that it is used in such an environment.

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment - Guidance
Conducted RF IEC 61000-4-6	3 Vrms 150 kHz to 80 MHz	[V1]= 3 V 150 kHz to 80 MHz and 6V at ISM Frequencies	Portable and mobile RF communications equipment should be used no closer to any part of the CS 8100 3D Family, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter. Recommended separation distance rf=[— b/p Γ1 d?=[—]-■/P 80 MHz to 800 MHz *Ei* *d* = [—]-*jp* 800 MHz to 2,5 GHz *Ei*
Radiated RF IEC 61000-4-3	3 V/m 80 MHz to 2.5 GHz	[E1]= 3 V/m 80 Mhz to 2.7 GHz	where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in metres (m). Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey should be less than the compliance level in each frequency range.b Interference may occur in the vicinity of equipment marked with the following symbol:

NOTE 1: At 80 MHz and 800 MHz, the higher frequency range applies.

NOTE 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

a Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which CS 8100 3D Family is used exceeds the applicable RF compliance level above, the CS 8100 3D Family should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the CS 8100 3D Family.

b Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Recommended Separation Distances between Portable and Mobile RF Communications Equipment and CS 8100 3D Family

The CS 8100 3D Family is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the CS 8100 3D Family can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the CS 8100 3D Family as recommended below, according to the maximum output power of the communications equipment.

Rated Maximum Output Power of Transmitter W	Separation Distance According to Frequency of Transmitter		
	150 kHz to 80 MHz	**80 MHz to 800 MHz**	**800 MHz to 2.5 GHz**
0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance d in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE 1: At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

NOTE 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

Compliance with International Regulations

- Medical Device Directives 93/42/EEC, Class IIb as amended by 2007/47/EC.
- Directive 2011/65/EU on the Restriction Of the use of certain Hazardous Substances in electrical and electronic equipment (RoHS).
- FDA Center for Devices & Radiological Health:

  CS 8100 3D: This product is in conformity with performance standards for diagnostic X-ray systems and their major components under 21 CFR 1020.30, and for computed tomography equipment under 21 CFR 1020.33, except with respect to those characteristics authorized by Variance Number FDA-2014-V-0657 effective 2014-07-15 (USA).

  CS 8100 3D Access: This product is in conformity with performance standards for diagnostic X-ray systems and their major components under 21 CFR 1020.30, and for computed tomography equipment under 21 CFR 1020.33, except with respect to those characteristics authorized by Variance Number FDA-2015-V-0980 effective 2015-05-28 (USA)
- Radiation Emitting Devices Act - C34 (Canada).
- Medical Devices Regulations (Canada).

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

3 Technical Specifications

Factory

TROPHY

4, rue F. Pelloutier, Croissy-Beaubourg

77435 Marne la Vallée Cedex 2, France

Manufacturer

Carestream Health, Inc.

150 Verona Street

Rochester, NY USA 14608

Model

CS 8100 3D

CS 8100 3D Access

CS 8100SC 3D

CS 8100SC 3D Access

CS 8100 3D Family Technical Specifications

Table 2 CS 8100 3D Family Technical Specifications

Components	CS 8100 3D / CS 8100 3D Access CS 8100SC 3D / CS 8100SC 3D Access
X-ray Generator	
Tube voltage	60-90 kV
Tube current	2-15 mA
Frequency	140 kHz
Tube focal spot (IEC 60336)	0.7 mm with X-ray tube OPX110 0.6 mm with X-ray tube D-067
Total filtration	> 2.5 mm eq. Al
Anode voltage	90 kV
Cathode current	15 mA

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Components	CS 8100 3D / CS 8100 3D Access CS 8100SC 3D / CS 8100SC 3D Access
Panoramic Modality	
Sensor technology	CMOS
Image field	6.4 x 140 mm (Adult) 6.4 x 120 mm (Pediatric)
Gray scale	16384 - 14 bits
Magnification	1.2
Radiological exams	Full panoramic Segmented panoramic Maxillary sinus Lateral TMJ x 2 Lateral TMJ x 4
Exposure mode	4 patient sizes (child, small adult, medium adult, large adult) 3 dental arch morphology (normal, square, sharp)
Exposure time	2 to 14 s
3D Modality	
Technology	Dental Volumetric Reconstruction (DVR)
Sensor technology	CMOS
Volume Field Of View (FOV) diameter x height (cm)	4 x 4 5 x 5 8 x 5 (optional for CS 8100 3D Access and CS 8100SC 3D Access) 8 x 8 (optional for CS 8100 3D Access and CS 8100SC 3D Access) 8 x 9* (optional for CS 8100 3D Access and CS 8100SC 3D Access)
Radiological exams	Full, upper or lower jaw Full, upper or lower molar Maxillary sinus Occlusion Focused teeth
Gray scale	16384 - 14 bits
Magnification	1.4
Voxel Size	75 µm minimum
Scan mode	Continuous
Exposure time	3 to 15 s
Reconstruction time	Less than 2 minutes based on the recommended computer system configuration requirements

* In Ontario (Canada), the use by dentists, of FOVs that are over 8 x 8, is subject to conditions

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Components	CS 8100 3D CS 8100 3D Access	CS 8100SC 3D CS 8100SC 3D Access
Cephalometric Modality		
Sensor technology	N/A	CMOS
Image field	N/A	6.4 x 263.3 m
Gray scale	N/A	16384 – 14 bits
Magnification	N/A	1.13
Radiological exams	N/A	Lateral Frontal AP or PA Oblique Submento-vertex Carpus (optional)
Exposure time	N/A	2.9 to 11 s
Input voltage (AC)	100-240 V - 50/60 Hz	
Unit dimensions	330 (L) x 894 (D) x 1596 (H) mm	1842 (L) x 936 (D) x 1596 (H) mm
Minimum required Space	1200 (L) x 1400 (D) x 2400 (H) mm	2000 (L) x 1400 (D) x 2400 (H) mm
Weight without the cephalostat component	92 kg (202 lb)	
Weight of only the cephalostat components	N/A	35 kg (77 lb)
Total weight	92 kg (202 lb)	127 kg (280 lb)

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Minimum Computer System Requirement

The computer and the peripheral equipment must conform to the IEC 60950 standard.

Item	Viewing	Acquisition
CPU	2 GHz Intel Duo Core	2,4 GHz Intel Duo Core
RAM	4 GB	8 GB
Hard disk drive	▪ 1.2 GB for software installation ▪ 250 GB free space to use the software	▪ 4 GB for software installation ▪ 500 GB free space to use the software
Graphic board	Nvidia/ATI based board supporting Open GL 1.2 with 512 MB of dedicated video RAM on AGP x8 video bus	▪ Cuda version 6.5 or higher ▪ Compute capability 1.1 or higher ▪ Nvidia based board on PCI Express video bus with minimum 2 GB of video RAM
Display	1024 x 768 minimum screen resolution 32 bits color mode	1280 x 1024 minimum screen resolution 1/1000
Operating system	▪ Windows 7 (64 bits) ▪ Windows 8/8.1** (64 bits) ▪ Windows 10** (64 bits)	▪ Windows 7 (64 bits) ▪ Windows 8/8.1** (64 bits) ▪ Windows 10** (64 bits)
Ethernet interface	N/A	2 Ethernet interfaces: ▪ 1 Gbits Ethernet board for the connection with the unit* ▪ Another optional Ethernet board for a LAN connection
CD/DVD drive	A DVD-BURNER drive is required.	A DVD-BURNER drive is required.
Backup Media	Removable/portable, external hard disk drive	Removable/portable, external hard disk drive.
Mouse	A mouse with 2 buttons and a scroll wheel is required	A mouse with 2 buttons

* This must be the Ethernet board of the motherboard if the computer has several gigabit Ethernet boards.

** CS 8100 3D Family is not compatible with touch screen desktop

Note: Always use Microsoft Windows Update to make sure that the latest security patches are correctly installed.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

X-ray Dose Emission Information

Panoramic mode for CS 8100 3D and CS 8100 3D Access

Table 3 Dose information for Panoramic modality

	kV	76	73	72	68
	mA	10	10	8	8
		[redacted]	Patient size		
Radiological exam	**Area of interest**	[redacted]	**Medium**	**Small**	**Child**
		DAP* in mGy.cm.cm			
Full Panoramic	Incisors, molars and TMJ	128	112	83	51
Segmented Panoramic Anterior	Incisor	75	55	32	15
Segmented Panoramic Anterior and Posterior	Incisors, one molar block and TMJ	101	84	57	33
Segmented Panoramic Anterior and Posterior	Incisors and one molar block	96	79	53	30
Segmented Panoramic Posterior	One molar block and TMJ	42	35	25	16
Segmented Panoramic Posterior	Two molar blocks and TMJ	85	70	51	32
Segmented Panoramic Posterior	One molar block	37	30	22	13
Segmented Panoramic Posterior	Two molar blocks	75	60	44	27
Segmented Panoramic Bitewing	Two molar blocks	136	115	80	38
Segmented Panoramic Anterior and Posterior	Incisors and molars	118	103	75	46
TMJ x2	TMJ	24	20	14	9
TMJ x4	TMJ mouth open and mouth closed	48	40	28	18
Maxillary Sinus	Maxillary sinus	91	78	53	30

*DAP: Dose Area Product. The accuracy of DAP in the table above is +/-30 % when compared with the values that could be measured.

Note: The information in the table above may be subject to modification. Without notice or justification to those concerned.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

3D mode for CS 8100 3D and CS 8100 3D Access

Table 4 Dose information for 3D modality

	kV	85	84	84	80
	mA	5	4	3,2	2,5
		Patient size			
Radiological exam	**FoV**	**Large**	**Medium**	**Small**	**Child**
		DAP* in mGy.cm.cm			
Jaw	8x 9**	1502	1169	935	NA
Jaw	8x9** Fast	701	545	436	NA
One arch (Lower or Upper Jaw)	8x5	938	730	584	405
One arch (Lower or Upper Jaw)	8x5 Fast	437	340	272	189
Jaw	8x8	1366	1063	850	591
Jaw	8x8 Fast	637	495	396	275
Focused teeth	5x5 Fast	272	211	169	NA
Focused teeth	4x4 Fast	NA	NA	NA	80

	kV	85	84	84	80
	mA	8	6,3	5	4
		Patient size			
Radiological exam	**FoV**	**Large**	**Medium**	**Small**	**Child**
		DAP* in mGy.cm.cm			
Focused teeth	5x5	932	714	566	NA
Focused teeth	4x4	NA	NA	NA	276

*DAP: Dose Area Product. The accuracy of DAP in the table above is +/-30 % when compared with the values that could be measured.
** 8 x 9 FoV: In Ontario (Canada), the use by dentists, of FOVs that are over 8 x 8, is subject to conditions.

Note: The information in the table above may be subject to modification. Without notice or justification to those concerned.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Panoramic mode for CS 8100SC 3D and CS 8100SC 3D Access

Table 5 Dose information for Panoramic modality

	kV	76	73	72	68
	mA	8	8	6.3	6.3
		Patient size			
Radiological exam	**Area of interest**	**Large**	**Medium**	**Small**	**Child**
		DAP* in mGy.cm.cm			
Full Panoramic	Incisors, molars and TMJ	145	129	94	63
Segmented Panoramic Anterior	Incisor	85	63	37	20
Segmented Panoramic Anterior and Posterior	Incisors, one molar block and TMJ	115	96	65	41
Segmented Panoramic Anterior and Posterior	Incisors and one molar block	110	91	61	38
Segmented Panoramic Posterior	One molar block and TMJ	48	40	29	20
Segmented Panoramic Posterior	Two molar blocks and TMJ	97	81	59	40
Segmented Panoramic Posterior	One molar block	43	35	25	17
Segmented Panoramic Posterior	Two molar blocks	86	70	50	34
Segmented Panoramic Bitewing	One molar block	77	66	46	24
Segmented Panoramic Bitewing	Two molar blocks	155	132	92	47
Segmented Panoramic Anterior and Posterior	Incisors and molars	134	118	86	57
TMJ x2	TMJ	29	24	17	12
TMJ x4	TMJ mouth open and mouth closed	59	49	35	24
Maxillary Sinus	Maxillary sinus	103	90	61	37

*DAP: Dose Area Product. The accuracy of DAP in the table above is +/-30 % when compared with the values that could be measured.

Note: The information in the table above may be subject to modification. Without notice or justification to those concerned.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

3D mode for CS 8100SC 3D and CS 8100SC 3D Access

Table 6 Dose information for 3D modality

	kV	90	90	90	80
	mA	3.2	2.5	2	2
		Patient size			
Radiological exam	**FoV**	**Large**	**Medium**	**Small**	**Child**
		DAP* in mGy.cm.cm			
Jaw	8x9**	1509	1179	943	NA
Jaw	8x9 ★★ st	704	550	440	NA
One arch (Lower or Upper Jaw)	8x5	916	715	572	453
One arch (Lower or Upper Jaw)	8x5 Fast	427	334	267	211
Jaw	8x8	1347	1052	842	665
Jaw	8x8 Fast	628	491	393	310
Focused teeth	5x5 Fast	273	214	171	NA
Focused teeth	4x4 Fast	NA	NA	NA	92

	kV	90	90	90	90
	mA	5	4	3.2	2
		Patient size			
Radiological exam	**FoV**	**Large**	**Medium**	**Small**	**Child**
		DAP* in mGy.cm.cm			
Focused teeth	5x5	916	732	586	NA
Focused teeth	4x4	NA	NA	NA	249

*DAP: Dose Area Product. The accuracy of DAP in the table above is +/-30 % when compared with the values that could be measured.
** 8 x 9 FoV: In Ontario (Canada), the use by dentists, of FOVs that are over 8 x 8, is subject to conditions.

Note: The information in the table aboves may be subject to modification. Without notice or justification to those concerned.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

	kV	85	80	75	70
	mA	2	2	2	2
		Patient size			
Radiological exam	**FoV**	**Large**	**Medium**	**Small**	**Child**
		DAP* in mGy.cm.cm			
Jaw	8x9 ★★ w dose	174	154	134	NA
Jaw	8x8 Low dose	156	137	119	101
One arch (Lower or Upper Jaw)	8x5 Low dose	106	94	81	69
Focused teeth	5x5 Low dose	68	60	52	NA
Focused teeth	4x4 Low dose	NA	NA	NA	30

*DAP: Dose Area Product. The accuracy of DAP in the table above is +/-30 % when compared with the values that could be measured.
** 8 x 9 FoV: In Ontario (Canada), the use by dentists, of FOVs that are over 8 x 8, is subject to conditions.

Note: The information in the table above may be subject to modification. Without notice or justification to those concerned.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Cephalometric mode for CS 8100SC 3D and CS 8100SC 3D Access

Table 7 Patient Dose information for Cephalometric modality for Lateral exam

kV	90	87	86	82
mA	10	10	8	8

Program	Patient size			
	Large	Medium	Small	Child
	DAP* in mGy.cm.cm			
18x18 High resolution	16	15	12	11
18x18 Fast	7	6	5	5
18x24 High resolution	19	18	14	13
18x24 Fast	8	8	6	5
26x24 High resolution	28	26	20	18
26x24 Fast	12	11	9	8

*DAP: Dose Area Product. The accuracy of DAP in the table above is +/-30 % when compared with the values that could be measured.

Note: The information in the tables above may be subject to modification. Without notice or justification to those concerned.

Table 8 Patient Dose information for Cephalometric modality for Carpus exam

kV	74	72	72	68
mA	15	15	15	15

Program	Patient size			
	Large	Medium	Small	Child
	DAP* in mGy.cm.cm			
18x18 High resolution	16	15	15	13
18x18 Fast	7	6	6	6
18x24 High resolution	19	18	18	15
18x24 Fast	8	8	8	7
26x24 High resolution	27	25	25	22
26x24 Fast	12	11	11	9

*DAP: Dose Area Product. The accuracy of DAP in the table above is +/-30 % when compared with the values that could be measured.

Note: The information in the tables above may be subject to modification. Without notice or justification to those concerned.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Table 9 Patient Dose information for Cephalometric modality for Frontal AP / PA, Oblique and Submento-vertex exam

kV	90	87	86	82
mA	10	10	8	8

	Patient size			
Program	**Large**	**Medium**	**Small**	**Child**
	DAP* in mGy.cm.cm			
18x18 High resolution	18	16	13	12
18x18 Fast	8	7	6	5
18x24 High resolution	21	20	15	14
18x24 Fast	10	9	7	6
26x24 High resolution	30	28	22	20
26x24 Fast	14	13	10	9

*DAP: Dose Area Product. The accuracy of DAP in the table above is +/-30 % when compared with the values that could be measured.

Note: The information in the table above may be subject to modification. Without notice or justification to those concerned.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice


User Dose information

Stray radiation in Panoramic Mode

Stray radiation measures are highly dependent on environmental conditions, such as the composition of walls and their locations, therefore in certain circumstances the values may be significantly different.
The points of measurement used are at 0.5 m, 1.0 m and 2.0 m respectively from the central rotation axis.

Figure 3 Circular Points of Measurement

Points of measurement	
1	Circular Points of Measurement
2	Chin Rest Axis
3	Chin Rest

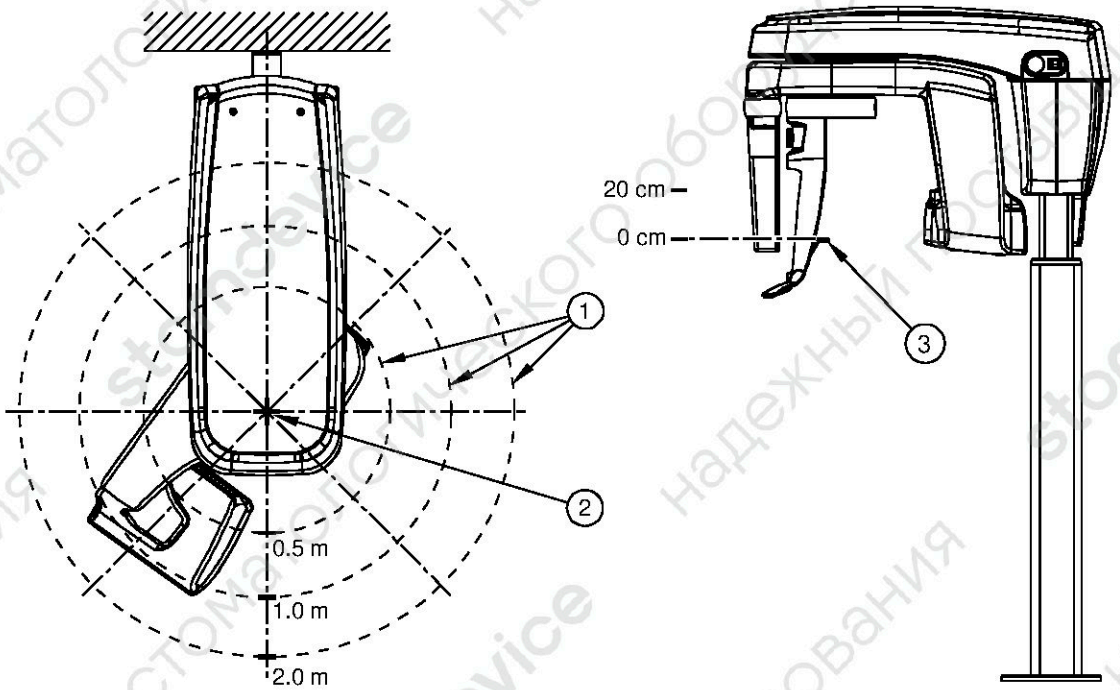

Stray radiation is measured in full panoramic mode, for a large sized patient selected with a PMMA phantom cylinder (Φ 16 cm, h 15 cm) to simulate a patient head.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

Stray radiation measured at the maximum use rate permitted by the X-ray generator, (this corresponds to a continuous average anodic power of 33 W), or 13 exams per hour.	
Distance between the rotation axis and measurement point (Circular Points of Measurement)	Stray radiation*
0.5 m	60 µGy /h
1.0 m	15 µGy /h
2.0 m	4 µGy /h
Stray radiation at mean use rate in practice, or 2 exams per hour.	
Distance between the chin rest axis and measurement point (Circular Points of Measurement)	Stray radiation*
0.5 m	8 µGy /h
1.0 m	2 µGy /h
2.0 m	< 1 µGy /h

*This is the maximum value measured 20 cm above the horizontal cross sectional plane with a chin rest. Other values in the vertical axis are lower than these values.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ


stomdevice

Stray radiation in 3D Mode

Stray radiation measures are highly dependent on environmental conditions, such as the composition of walls and their locations, therefore in certain circumstances the values may be significantly different.
The points of measurement used are at 0.5 m, 1.0 m and 2.0 m respectively from the central rotation axis.

Figure 4 Circular Points of Measurement

Points of measurement	
1	Circular Points of Measurement
2	Chin Rest Axis
3	Chin Rest

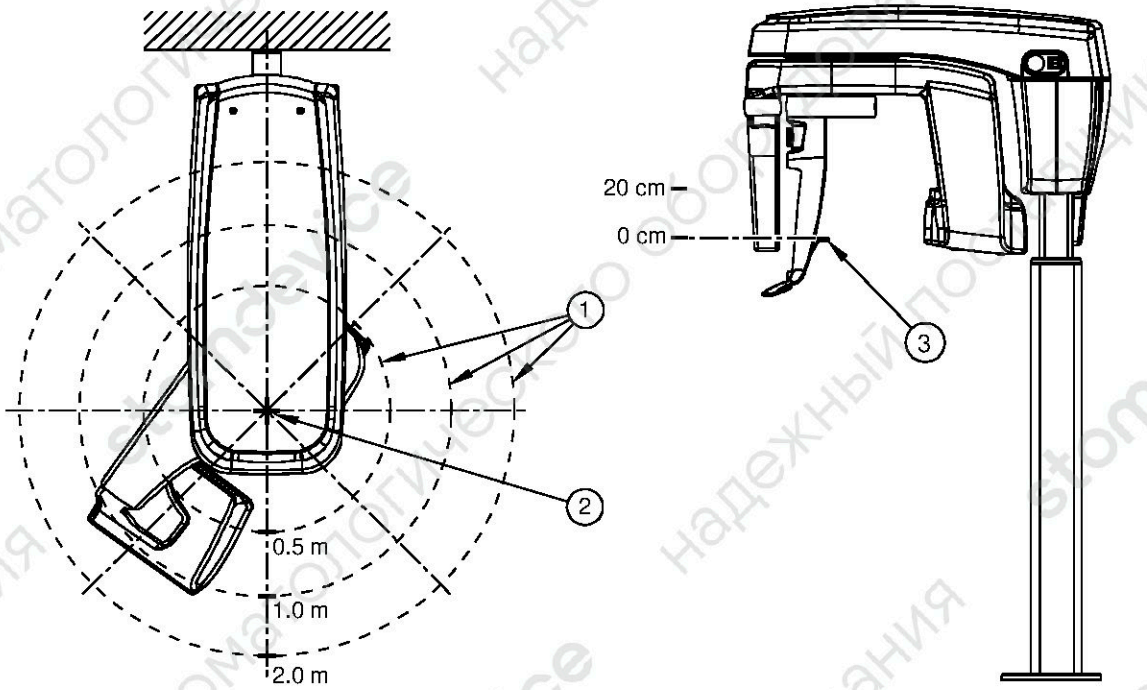

Stray radiation is measured in largest 3D mode available, ie 8x9 mode, for a large sized patient selected with a PMMA phantom cylinder (Φ 16 cm, h 15 cm) to simulate a patient head.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Stray radiation measured at the maximum use rate permitted by the X-ray generator, (this corresponds to a continuous average anodic power of 33 W), or 8 exams per hour.	
Distance between the rotation axis and measurement point (Circular Points of Measurement)	Stray radiation*
0.5 m	420 µGy /h
1.0 m	105 µGy /h
2.0 m	26 µGy /h
Stray radiation at mean use rate in practice, or 2 exams per hour.	
Distance between the chin rest axis and measurement point (Circular Points of Measurement)	Stray radiation*
0.5 m	108 µGy /h
1.0 m	27 µGy /h
2.0 m	7 µGy /h

*This is the maximum value measured 20 cm above the horizontal cross sectional plane with a chin rest. Other values in the vertical axis are lower than these values.

Imaging performance information

Panoramic and Cephalometric

Line Pair Resolution*: 3.1 lp/mm minimum.
Low Contrast Resolution*: a minimum of 2 low contrast steps for panoramic and a minimum of 1 low contrast step for cephalometric.
* Using a dental phantom for digital image acquisition that complies with the IEC 61223-3-4:2000 standard.

3D

The value of the Modulation Transfer Function** (MTF) at 10 % is superior to 1 lp/mm.
The Signal-to-Noise Ratio (SNR) measured in an homogeneous 1 mm thick slice of PMMA*** material is greater than 10.
** Using a dental phantom for digital image acquisition that complies with the DIN 6868-161 standard.
*** Polymethyl methacrylate (PMMA) is a transparent thermoplastic material.
The CS 8100 3D Family do not provide Computed Tomography (CT) numbers, therefore, conventional analyses using CT numbers cannot be made.

Controlling the Image Quality

For optimum results, perform a control test of the image quality. To do this, see "***Controlling the Image Quality***" chapter in the ***Panoramic and 3D Modality User Guide for CS 8100 3D Family, (SM842)***.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

CS 8100 3D Family Environmental Requirements

Ambient Operating Conditions	
Temperatures	10 – 35°C (50 – 95°F)
Relative humidity	30 – 80 %
Atmospheric pressure	700 – 1060 hpa
Altitude	Up to 3000 m

Storage Conditions	
Temperatures	-10 – 60°C (14 – 140°F)
Relative humidity	10 – 90 %
Atmospheric pressure	700 – 1060 hpa

Transport Conditions	
Temperatures	-10 – 60°C (14 – 140°F)
Relative humidity	10 – 90 %
Atmospheric pressure	700 – 1060 hpa

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

CS 8100 3D Family Electrical Specifications

Type of Electrical Power Supply	100 - 240 V ~ (± 10%) 50/60 Hz, Single-Phase
Acceptable fluctuation	± 10%
Apparent resistance of the power supply circuit	0.12 Ω max
Permanent absorbed current	1.0 A
Current absorbed during the X-ray emission	20 A
Maximum absorbed power	2.2 kVA
Protection for the power supply system	By shutter release at a maximum current of 20 A and a differential current of 30 mA
Nominal high voltage	90 kV
Maximum corresponding tube current	10 mA
Nominal tube current	15 mA
Maximum corresponding high voltage	80 kV
Tube current/voltage combination for maximum output power	80 kV, 15 mA, 1200 W
Nominal power for an exposure time nearest to 100 kV and to 0.1 s.	at 90 kV, 10 mA: 900 W

Selection of the Load Parameters:	
kV (in increments of 1 kV)	From 60 to 90 kV
mA (in increments of 25 %)	From 2 to 15 mA

Utilization Rate in Continuous Mode (for example: one exposure - 85 kV, 5 mA - 13.9 second, every 3 minutes)	Utilization Rate in Intermittent Mode (for example: one exposure - 80 kV, 15 mA - 13.9 second, every 3 minutes)
33 W	93 W

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Accuracy of the Load Parameters	
High voltage	kV ± 10 %
Current in the tube	mA ± 20 %
Exposure time seconds	Seconds ± (10 % + 1ms) or ± (5% + 50ms)

Measurement Conditions	
kV	Indirect on the peak kilovolt meter
mA	Direct measurement in the circuit using an oscilloscope
Exposure time	Measurement at 75 % of the kV values with peak kilovolt meter

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

X-ray Tube Assembly Technical Specifications


Table 10 Filtration of the Material in the X-ray Field

Standard	Compliant
IEC 60601-1-3	Compliant
Nominal value of the inherent filtration at 70 kV	>1.7 mm (0.07") eq. Al
Nominal value of the supplementary filtration at 70 kV	2.5 mm (0.10") eq. Al min
Nominal value of the total filtration at 70 kV	> 2.5 mm (0.10") eq. Al
Filtration value for the enclosure of the X-ray tube (at 100 kV)	0.5 mm (0.020") eq. Al
Filtration value for the sensor case (at 100 kV)	1 mm (0.039") eq. Al

The X-ray generator comprises the following:

- Transformers and an X-ray tube and their associated electronic components immersed in oil
- Copper filter (for CS 8100 3D and CS 8100 3D Access) or Copper + Aluminum filter (for CS 8100SC 3D and CS 8100SC 3D Access), which enhances the quality of the beam and reduces the dose received by the patient
- A lead collimator, which limits the size of the beam at the image receiver unit
- A thermal cutout, which trips at an operating temperature between 63 to 70 °C (± 5°C)

Figure 5 Location of the Reference Axis for Panoramic and 3D Imaging

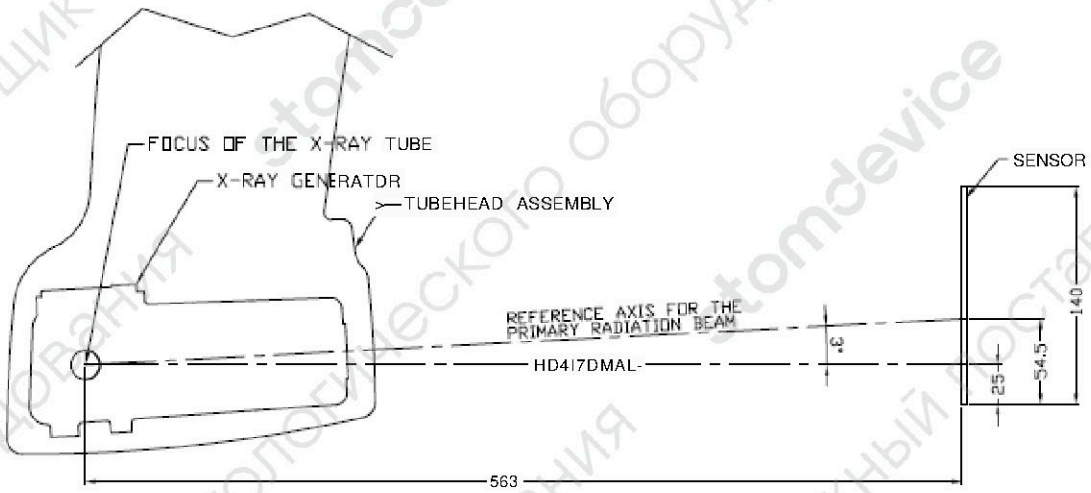

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Figure 6 Location of the Reference Axis for Cephalometric Imaging

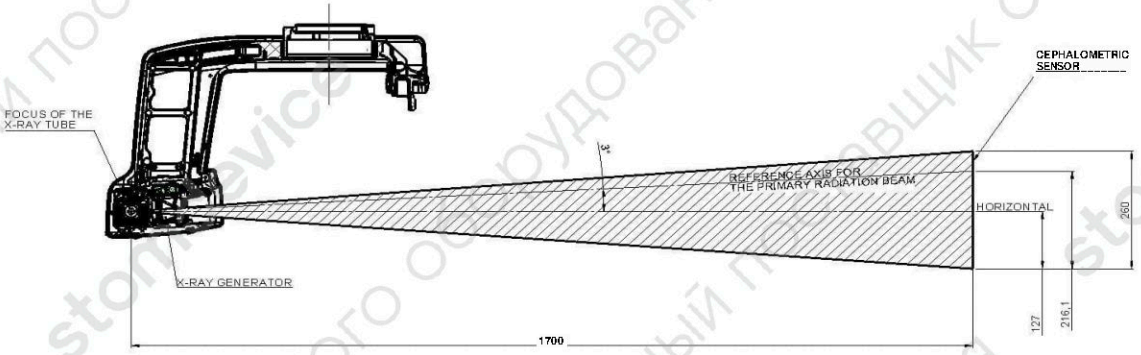


Table 11 Technical Specifications of the X-ray tube Assembly

Standard	Compliant
Manufacturer	Trophy
Degree of protection against electric shock	Class I
Degree of patient protection from the parts applied to the leakage current	Type B
Operation mode	Continuous operation with intermittent loading
Maximum accumulated heat	110 kJ
Maximum continuous heat dissipation	33 W
Nominal value of the focal spot	0.7 mm with X-ray tube OPX 110 0.6 mm with X-ray tube D-067
Tolerances on the position of the focal spot	± 2.5 mm
Continuous Anode Input Power that corresponds to the maximum specified energy input to the Anode (110 kJ)	33W at 90kV
Radiation leakage after one hour's operation (maximum utilization rate of 33W)	< 1 mGy
Weight	7 kg
Dimensions	270 x 200 x 100 mm

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Figure 7 Heating and Cooling Curves of the X-ray Tube Assembly

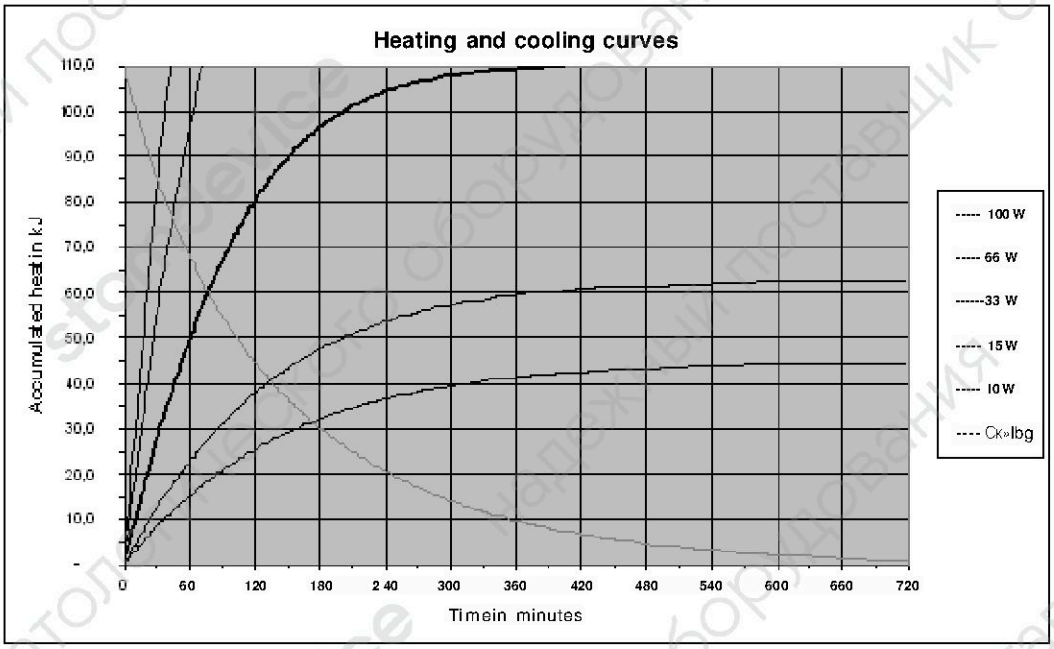


Table 12 Beam Limitations of the X-ray Tube Assembly

Manufacturer	Trophy
Type	Rigidly mounted unit with fixed window dimensions, not removable, and integrated X-ray generator
Maximum symmetrical field of radiation in panoramic mode at a distance of 563 mm from the focal point	5 mm x 140 mm At the detector reference plane
Maximum symmetrical field of radiation in 3D mode at a distance of 563 mm from the focal point	120mm x 140mm At the detector reference plane
Maximum symmetrical field of radiation in cephalometric mode at distance of 1700 mm from the focal point	5 mm x 260 mm At the detector reference plane
Location of the reference axis	See Figure 5 and Figure 6Location of the Reference Axis for Panoramic and 3D Imaging

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Table 13 Characteristics of the X-ray Tube

Manufacturer's name	CEI	Toshiba
Type	OPX110	D-067
Nominal high voltage	110 kV	100 kV
Nominal anode input power at 0.1 s (AC)	1755 W	1260 W
Anode heat storage capacity	30kJ	35 kJ
Nominal focal spot size (IEC 60336)	0.7 mm	0.6 mm
Anode materials	Tungsten	Tungsten
Target angle	12°	12°
Inherent filtration	0.5 mm (0.020 ") eq. Al	0.8 mm (0.032'') eq. Al

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Figure 8.1 X-ray tube drawing OPX110


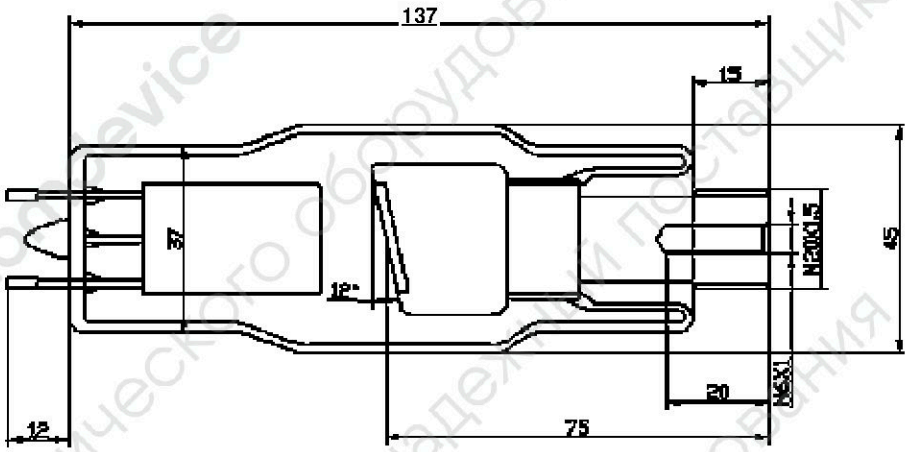


Figure 8.2 X-ray tube drawing D-067

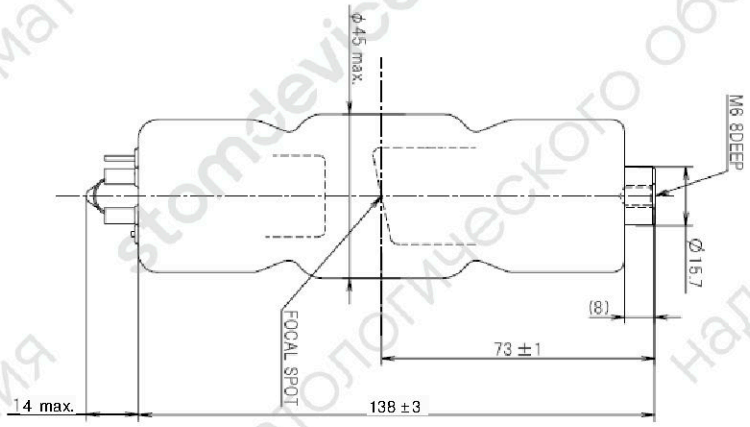

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Figure 9.1 Heating and Cooling Curves of the X-ray Tube OPX110


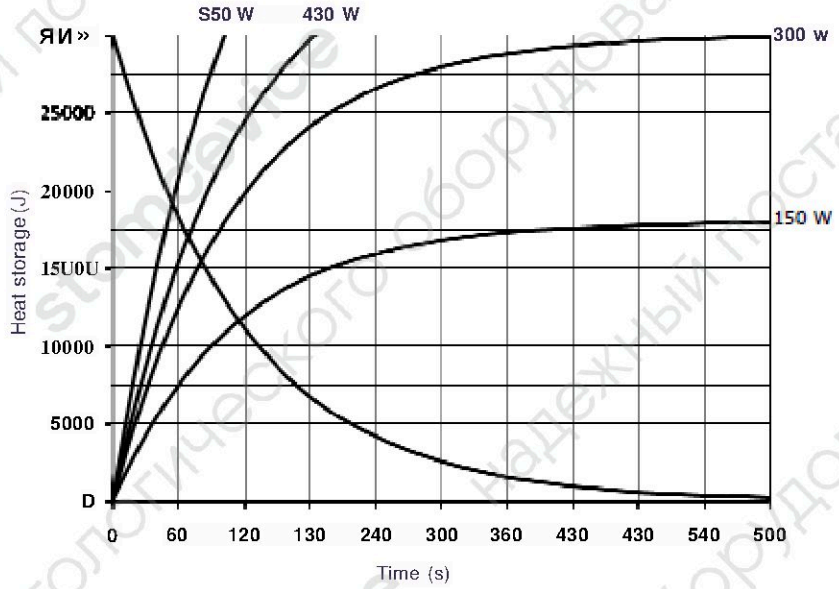


Figure 9.2 Heating and Cooling Curves of the X-ray Tube D-067

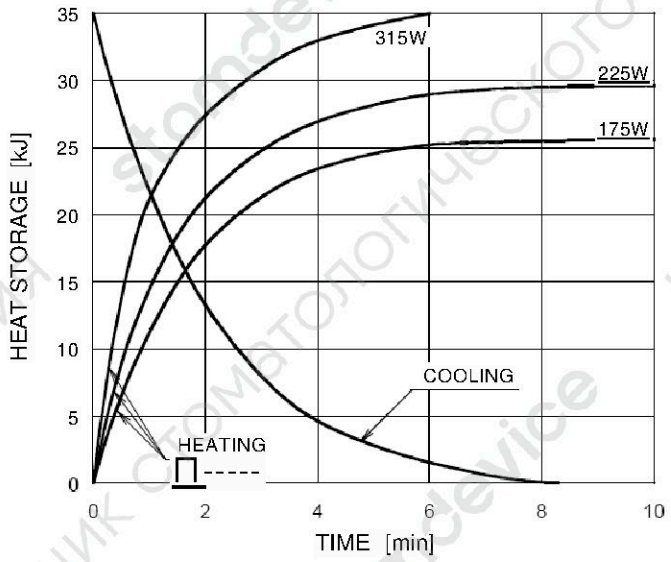

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Figure 10.1 Single Load Chart of the X-ray Tube OPX110


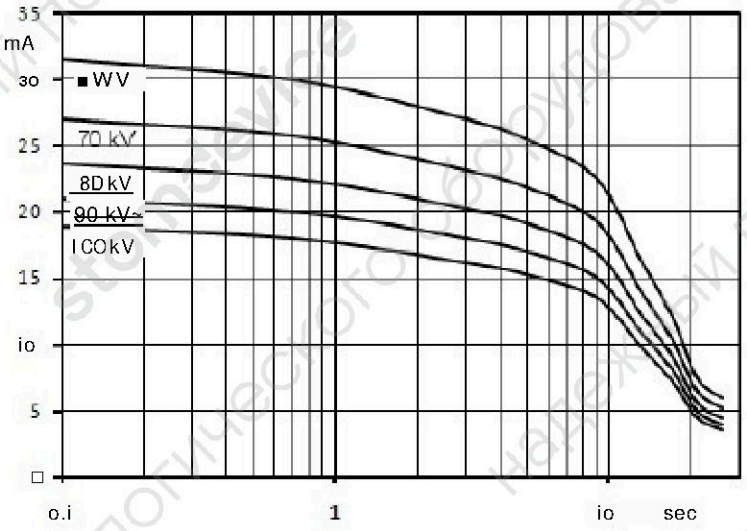


Figure 10.2 Single Load Chart of the X-ray Tube D-067

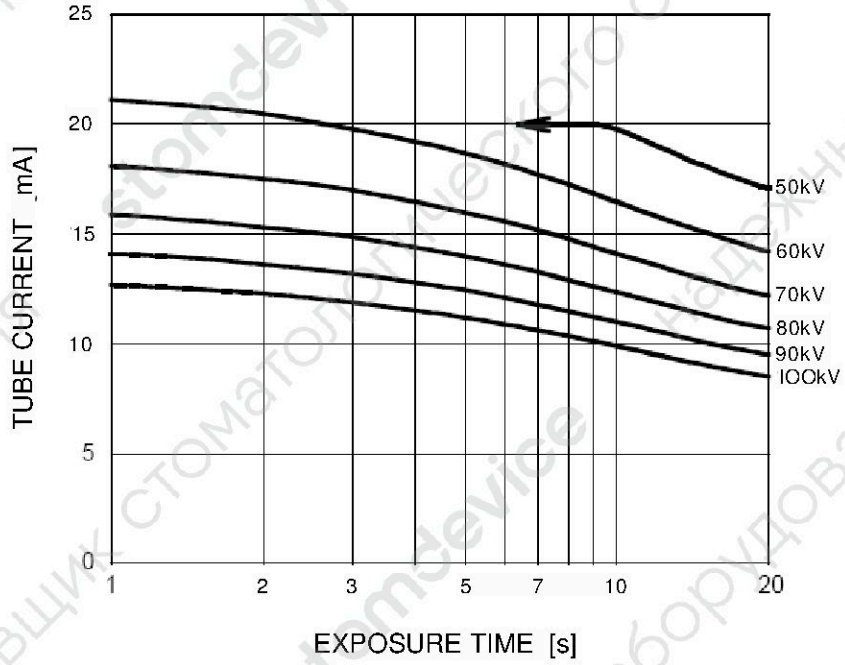

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Figure 11.1 Filament Emissions of the X-ray Tube OPX110


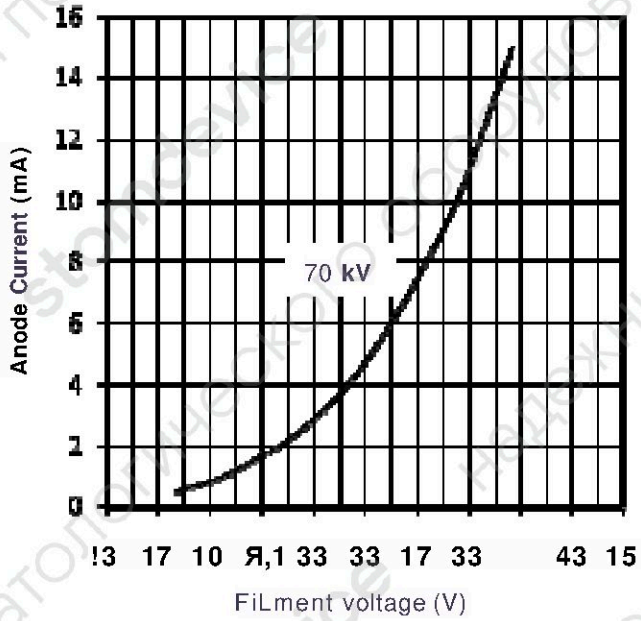


Figure 11.2 Filament Emissions of the X-ray Tube D-067

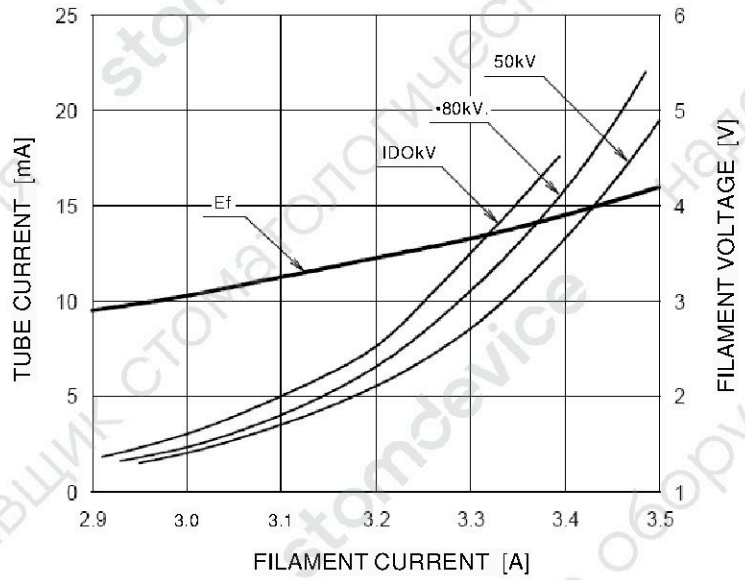

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

4 Contact Information

Manufacturer's Address



Carestream Health, Inc.
150 Verona Street
Rochester, NY, USA 14608

Factory

Trophy

4, Rue F. Pelloutier, Croissy-Beaubourg

77435 Marne la Vallée Cedex 2, France

Authorized Representatives

Authorized Representative in the European Community

EC REP

Carestream Health France

1, rue Galilée

93192 Noisy-Le Grand Cedex, France

Representante no Brasil Carestream do Brasil Comércio e Serviços de Produtos MédicosLtda.

Rua Pequetita, 215 cjs.
31 E 32 Edifício Atrium VII - Vila Olímpia
São Paulo - Brazil
CEP (Zip code): 04552-060

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Carestream Dental
A Division of Carestream Health, Inc.
150 Verona St.
Rochester, NY 14608
USA

For more information, visit: **www.carestreamdental.com**
To give documentation feedback, visit:
www.carestreamdental.com/documentationfeedback

©Carestream Health, Inc., 2016
SM844 Ed08 2016-09
https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ