stomdevice




Clair
Owner´s Manual

D-TEC
LIGHTING SYSTEMS

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

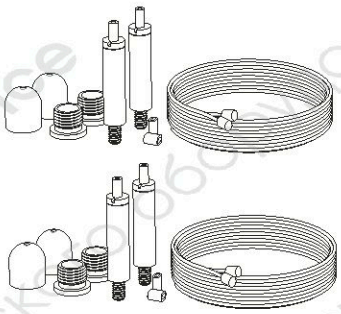





Note: Don´t use sharp objects when unpacking the luminaire!

1. Unpacking Your Clair


Carefully open the packaging without using any sharp objects!

In the packaging you will find the following items:


- Wire arrangements for attaching the luminaire to the ceiling. (4 pcs)
- The Clair Luminaire
- Remote Control Unit and holder

D-TEC LIGHTING SYSTEMS


https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

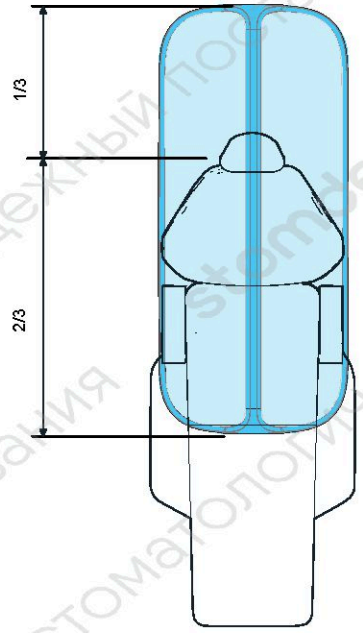


Parallell position. The eyes of the patient should be in line with 1/3rd of the luminaire.

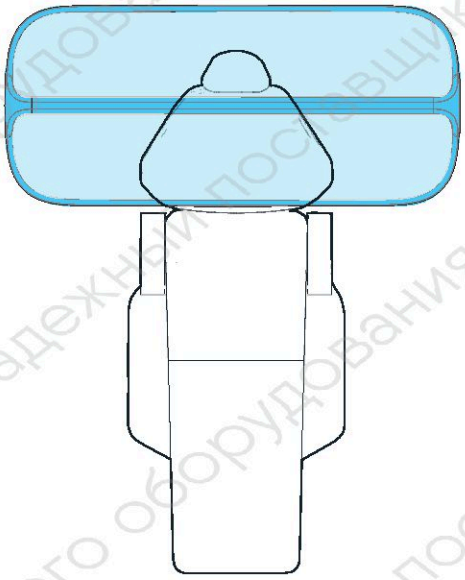

Crosswise position.

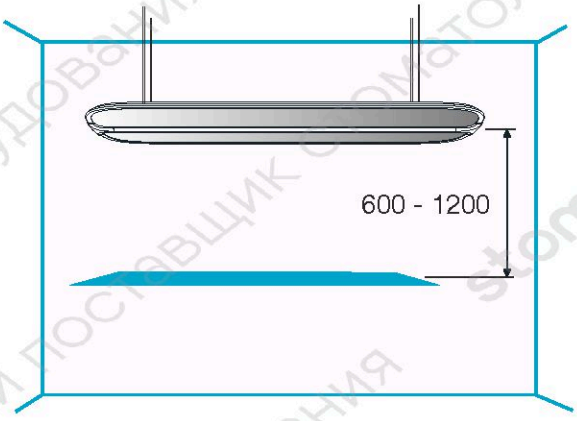

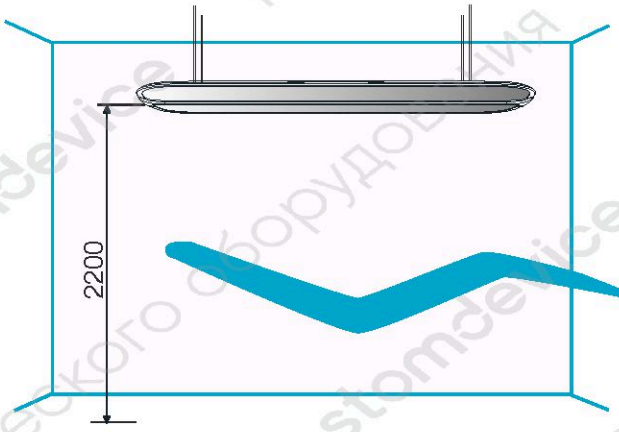


2. Positioning Your Clair

The height of the luminaire should be about 600 - 800mm above the working area.


https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice



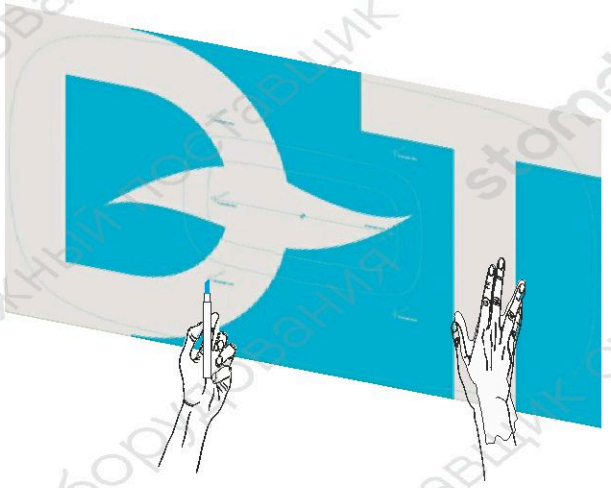



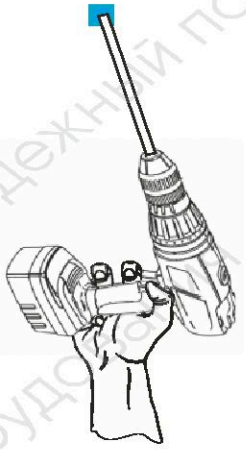

3. Preparing the mounting of Your Clair


AFTER unpacking the luminaire you can use the packaging as a guide for marking the attachment points in the ceiling.


• Use the front part of the packaging and punch holes with a screw-driver or similar.


• Position the cardboard lid where you want to mount the luminaire, mark out the ceiling points and drill your holes for the attachment.


D-TEC LIGHTING SYSTEMS

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

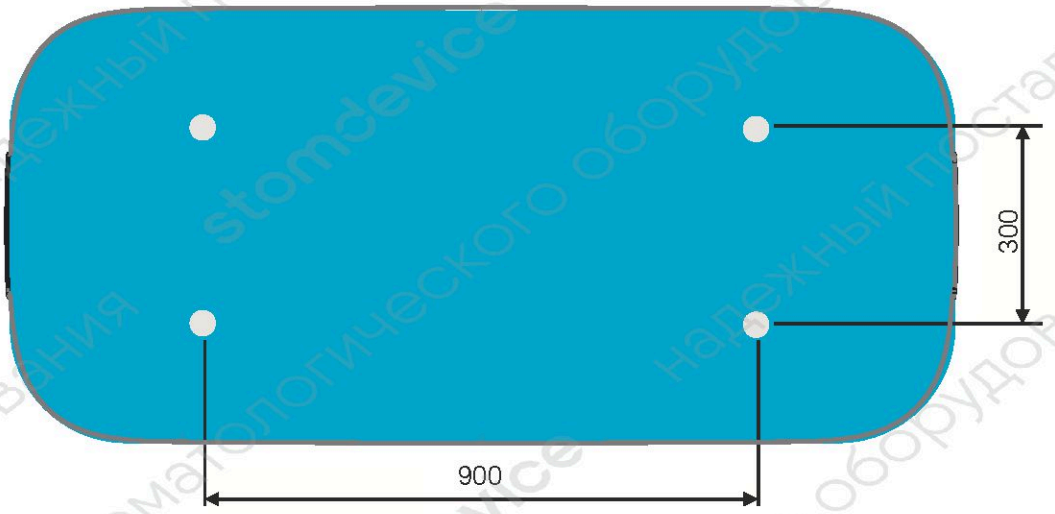

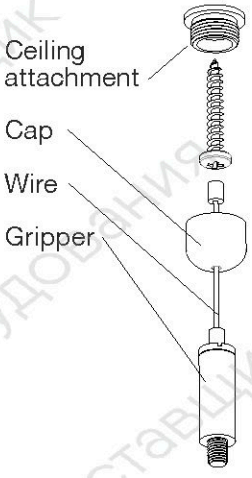

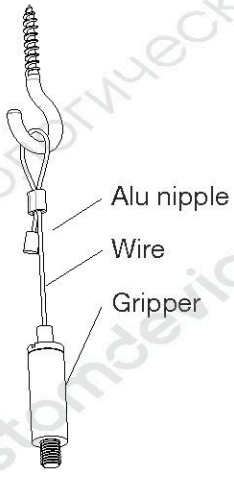


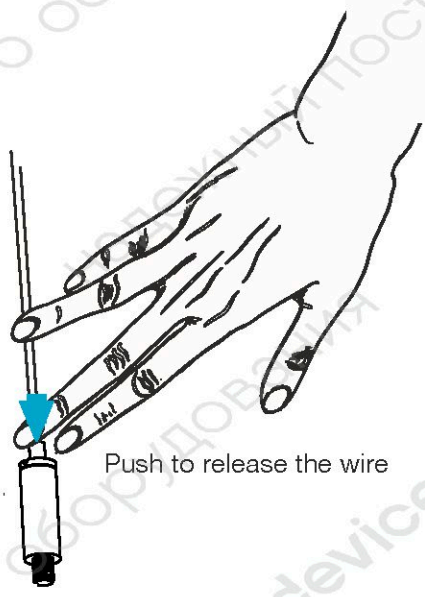

4. Mounting Your Clair in the ceiling

These items for mounting are provided with the luminaire. Use the one suitable for your needs.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

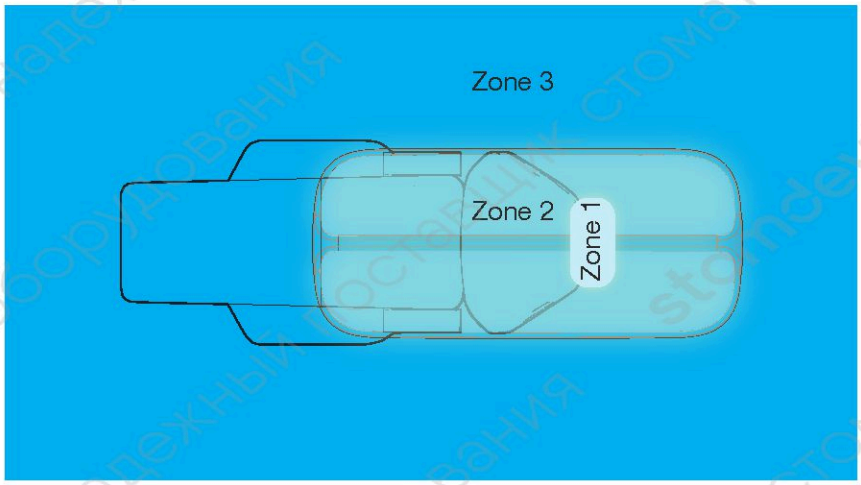

5. Light conditions for surgery

Image of preferred light conditions for operation rooms.


Zone 1 = 20 000 - 30 000 LUX

Zone 2 = 3000 - 5000 LUX

Zone 3 = 500 - 1000 LUX

Caution!

Fade out the lamp when working with light/curing materials.

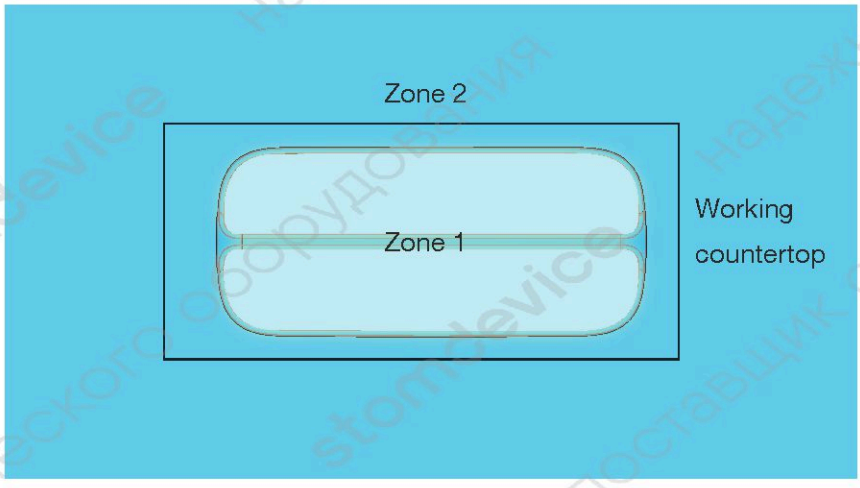


6. Light conditions for examination

Image of preferred light conditions for examination rooms.

Zone 1 = 3000 - 5000 LUX

Zone 2 = 500 - 1000 LUX

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

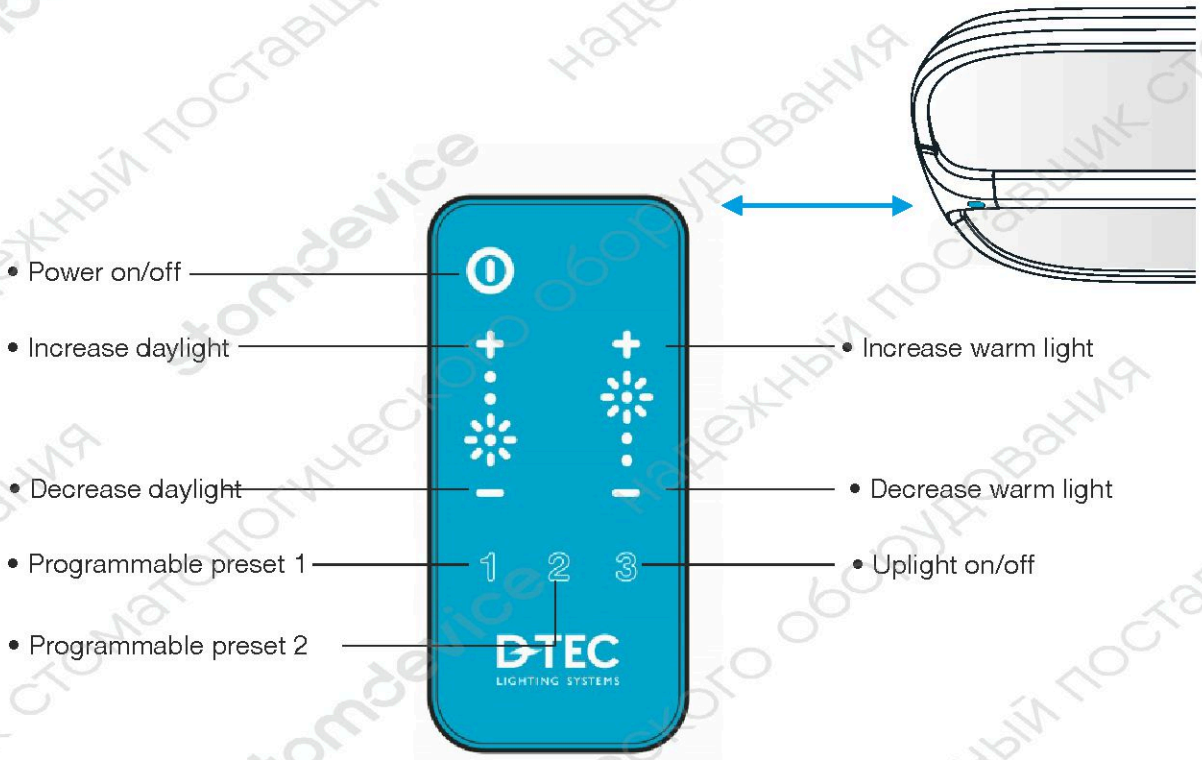


7. Operating Your Clair with the remote control unit


The Clair luminaire is equipped with a remote control for all functions. This remote control is delivered with a holder that could be mounted on a wall, table etc.

When working with light curing materials (composite) it can be an advantage to decrease the daylight since it can make your material cure too fast. Lowering the daylight in Clair will also make it easier to examine x-rays. The luminaire has two presets programmed from factory, and you can modify these presets at any time:
Set the desired light mix with the +/- buttons and button 3 for uplight. Hold buttons 1 or 2 for approx 3 seconds. The sun symbol on the luminaire will flicker to indicate that the new program has been stored.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

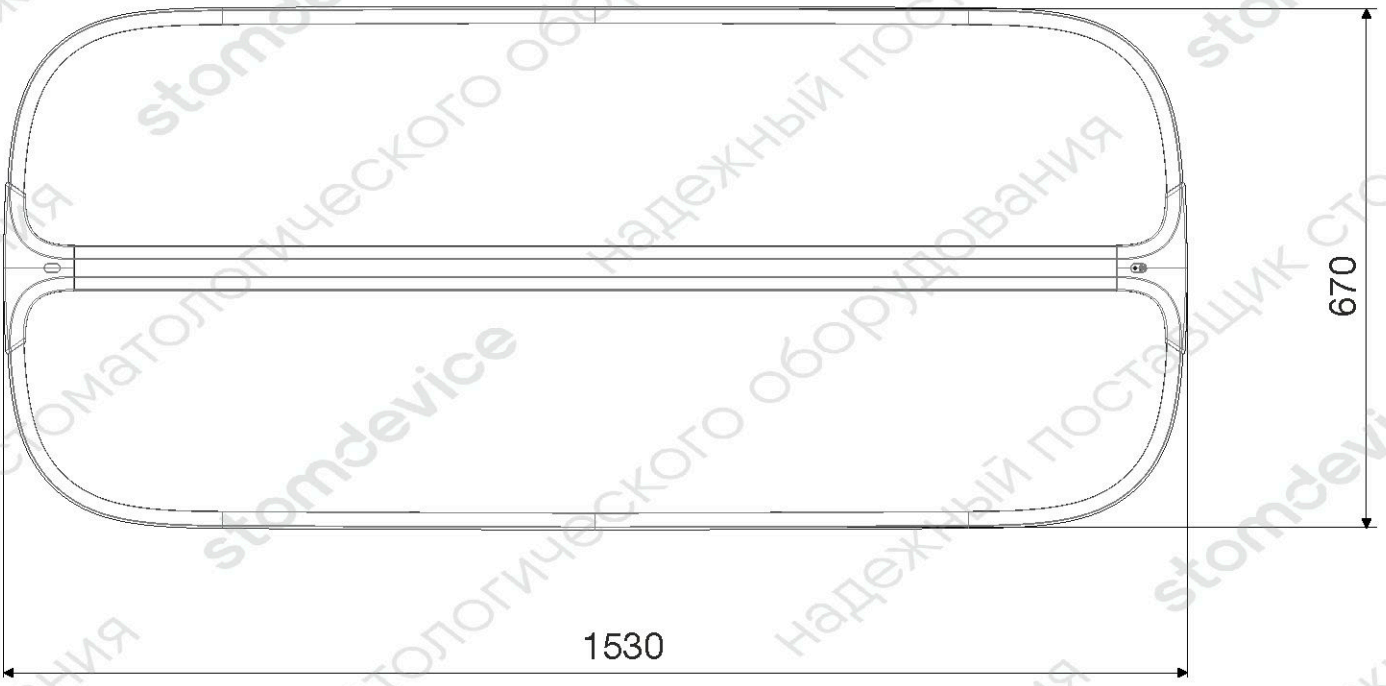



D-TEC LIGHTING SYSTEMS

9. Clair dimensions

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

On-line support:
http://d-tec.se/support

- Bruksanvisning
- Manuel d'utilisation
- Bedienungsanleitung

D-TEC
LIGHTING SYSTEMS

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Facts: Clair CL104

- High power - 200-3000Lux/1.2m
- Up to 21325 Lumen
- 230V
- 3000-6500K CRI (Ra) 86-93
- Dimmable
- Energy saving
- Remote control
- Size: 1530x670x59
- Weight: 16,3kg

D-TEC AB
Varavägen 12
SE-465 94 Nossebro
Phone: +46 (0)31-96 93 02 Fax: +46 (0)31-96 60 92
E-mail: mailbox@d-tec.se
www.d-tec.se

D-TEC LIGHTING SYSTEMS

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ