
stomdevice

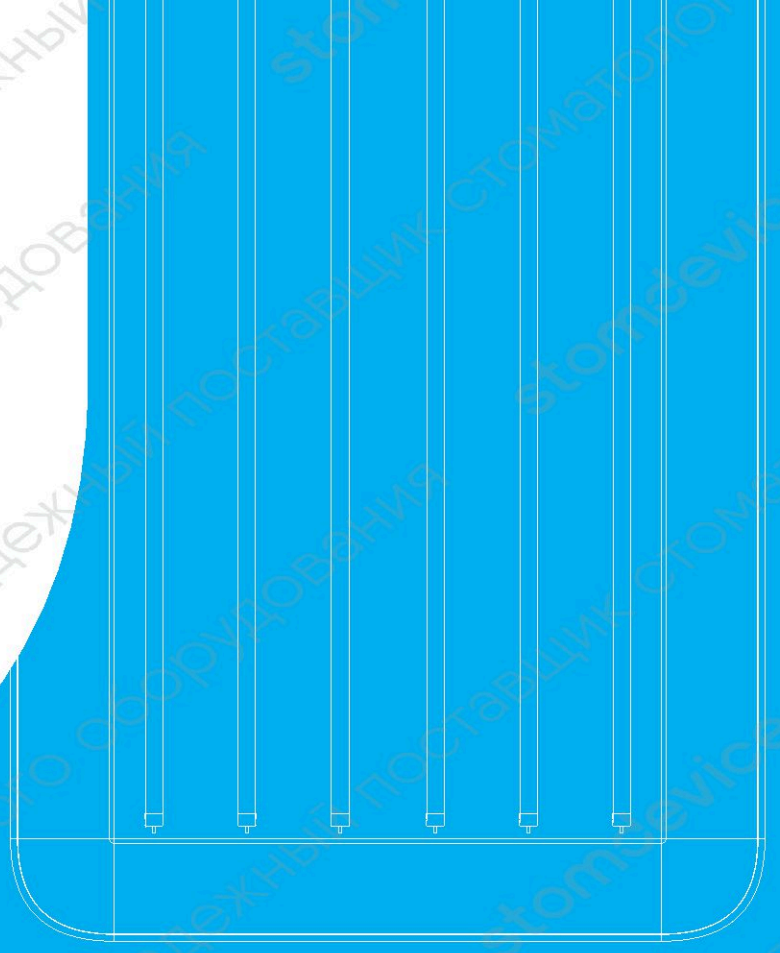



Denta/Dentaplus
Owner´s Manual

D-TEC
LIGHTING SYSTEMS

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

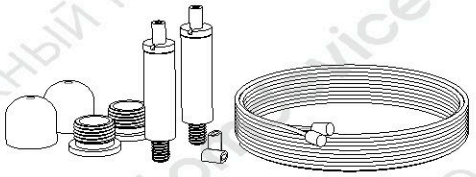

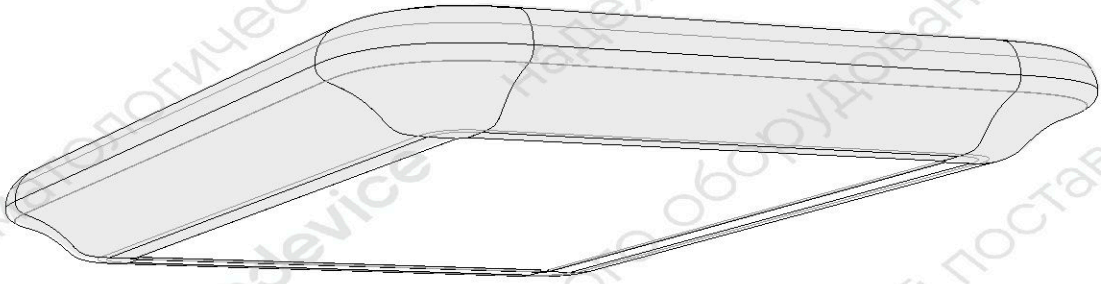

Note: Do not use sharp objects when unpacking the luminaire!

1. Unpacking your Denta/Dentaplus


Open the packaging carefully without using any sharp objects!


The packaging includes:


- Wire arrangements for attaching the luminaire to the ceiling (4 pieces)
- The Denta/Dentaplus luminaire


D-TEC LIGHTING SYSTEMS

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

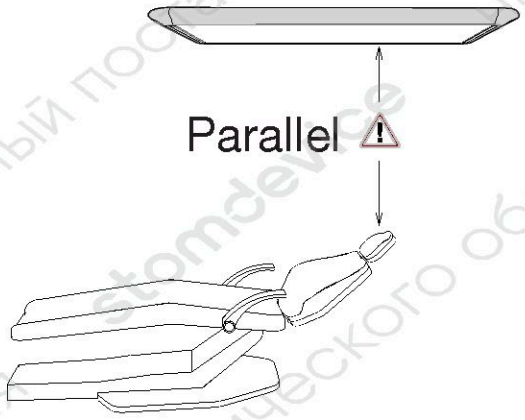

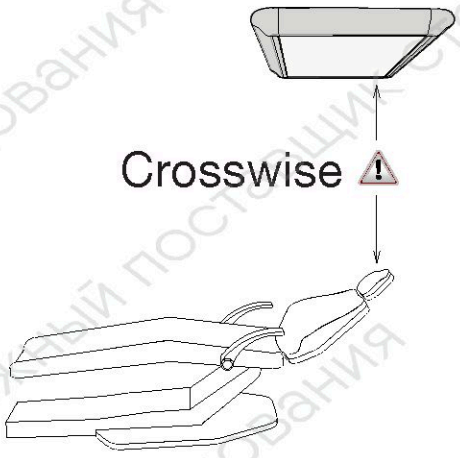

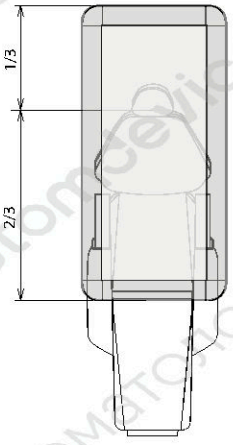

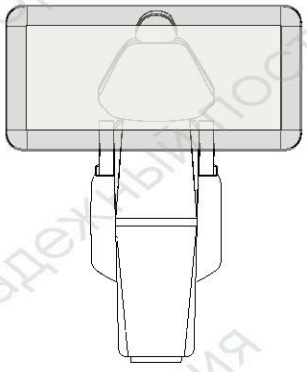


2. Positioning your Denta/Dentaplus

The luminaire should be positioned in one of the following two positions:


- Parallel position - the eyes of the patient should be in line with 1/3rd of the luminaire.
- Crosswise position - the eyes of the patient should be in line with the top of the light source.


Note: The recommended height of the luminaire is to be placed 2,2 meters above floor level

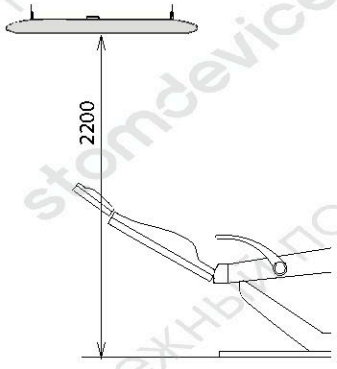

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

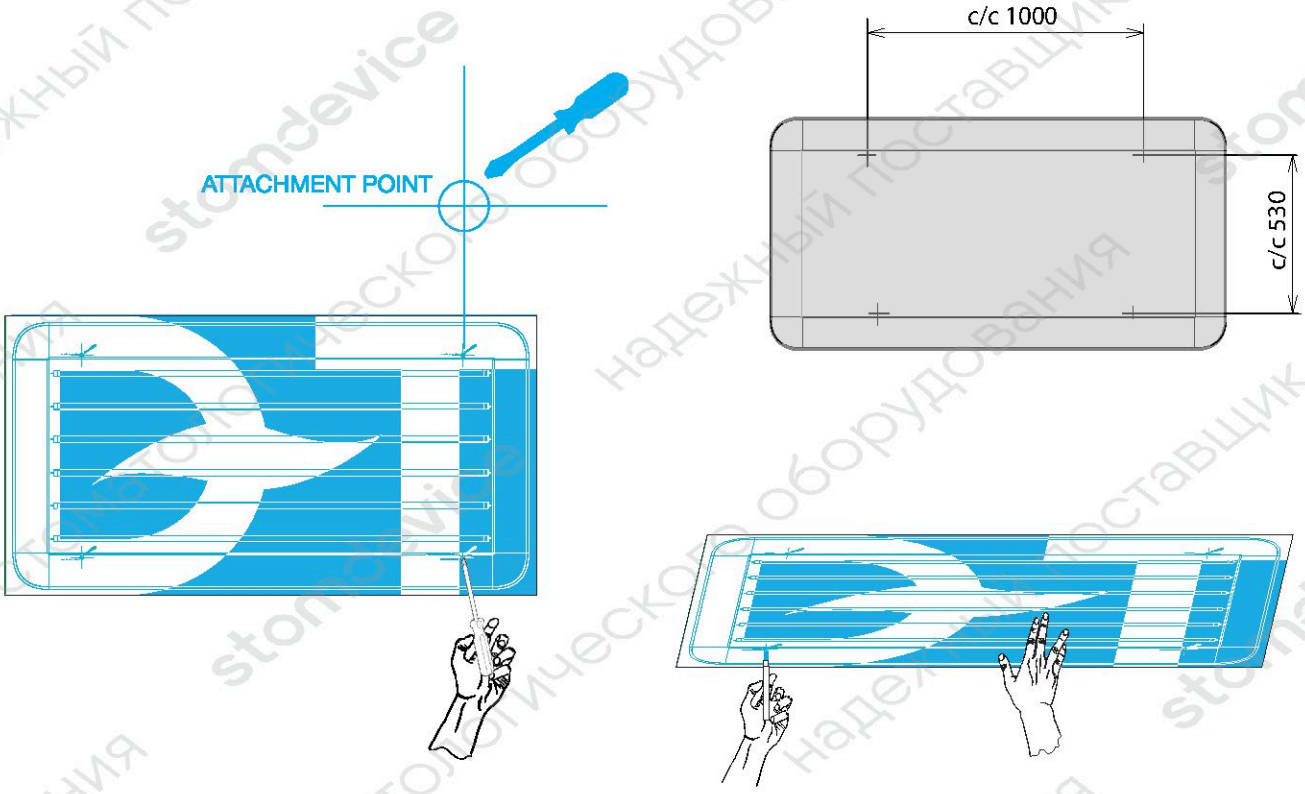

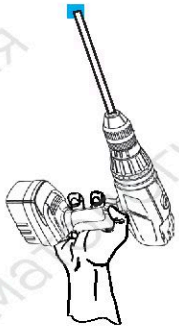

3. Preparing the mounting of your Denta/Dentaplus


After unpacking the luminaire use the packaging as a guide for marking the attachment points in the ceiling.


• On the outside of the cardboard, there are four attachment points marked out. Punch a hole in these four points with a screwdriver or similar.

• Hold the cardboard lid where you want to position the luminaire in the ceiling and mark the four points where you would like the wires to be attached and drill holes accordingly

D-TEC LIGHTING SYSTEMS

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

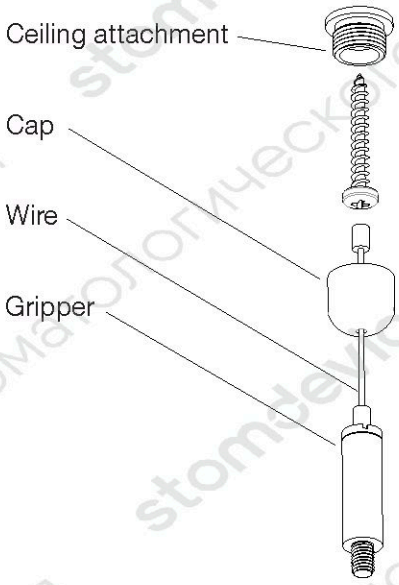

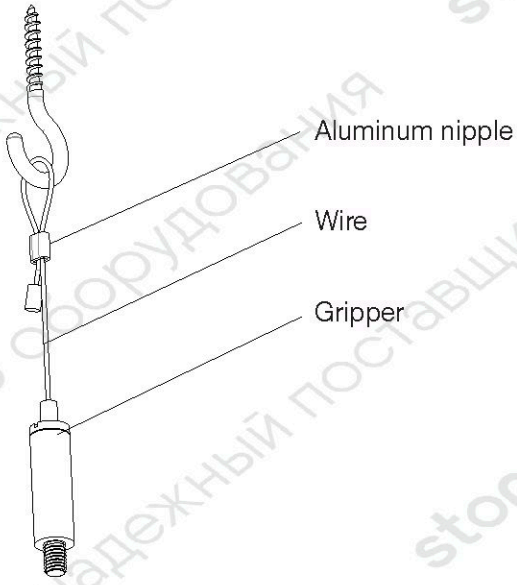


4. Mounting your Denta/Dentaplus in the ceiling

There are two options of mounting kits enclosed with your luminaire.

Use the kit suitable to your needs and preferences.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

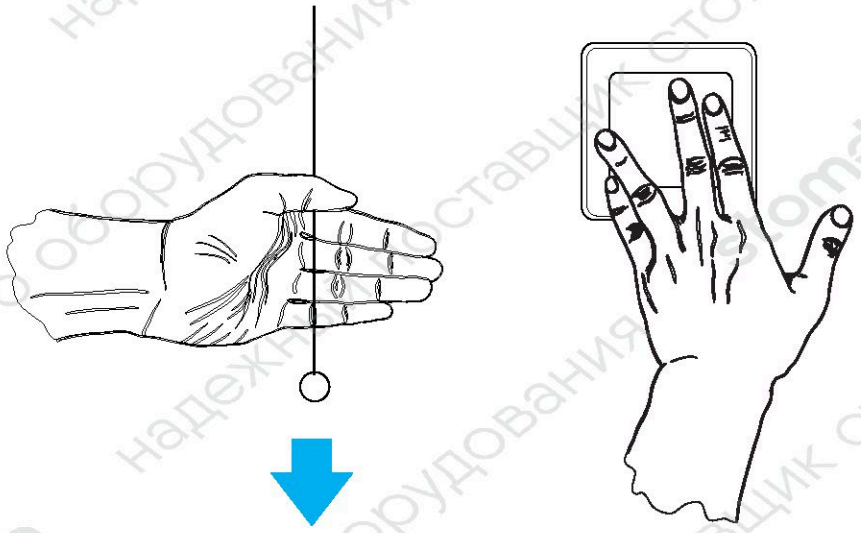

5. Operating your Denta luminaire


The luminaire is operated by a pulling string/cord or, on special requests, by a wall switch. The luminaire could be faded in such a way that the two middle sections of lights are switched off by a pull of the string.


The indirect light is optional and will always be unchanged/constant.

Caution! Ensure you fade out the lamp when working with lightcuring materials.

D-TEC LIGHTING SYSTEMS

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

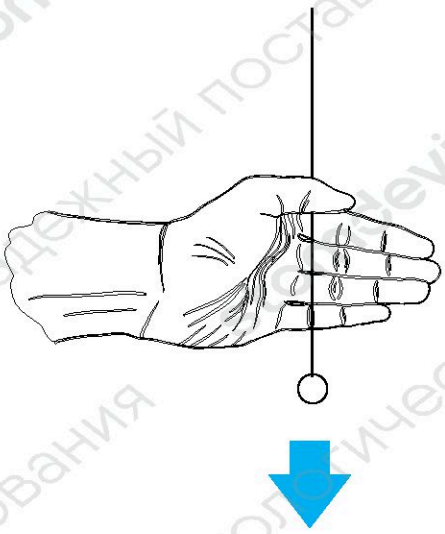

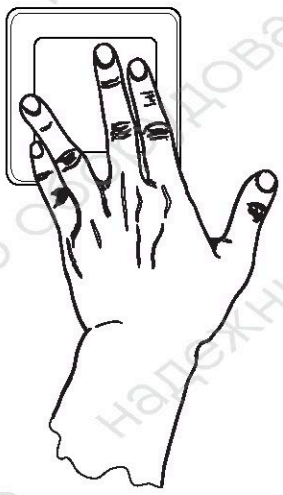

6. Operating Your Dentaplus luminaire

The luminaire is operated by a pulling string/cord or, on special requests, by a wall switch. Instructions to operate the dimmer function:

- Switching the lamp on/off: short pull (<0,5 second)
- Dimming: Long pull (>0,5 second), the dimming direction is changed with each pull.
- To reset: pull and hold the string for approximately 30 seconds


The last dimmer setting is remembered until the next time the luminaire is switched on.

The indirect light is optional and will always remain at the same brightness, that is, unchanged/constant and not affected by the dimming device.

Caution! Ensure you fade out the lamp when working with lightcuring materials.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

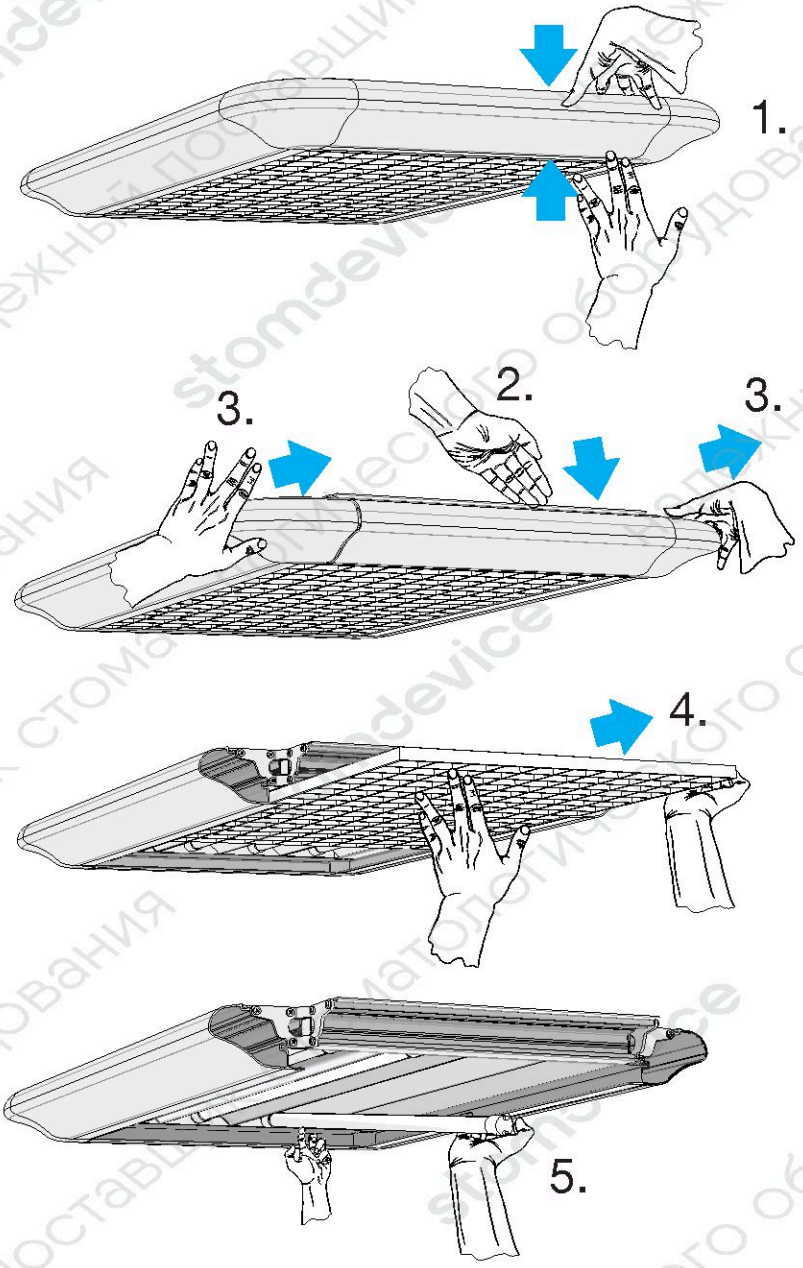


7. Exchange of fluorescent light tubes

- Denta: 6 x 28 W
- Dentaplus: 6 x 54 W

D-TEC LIGHTING SYSTEMS

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

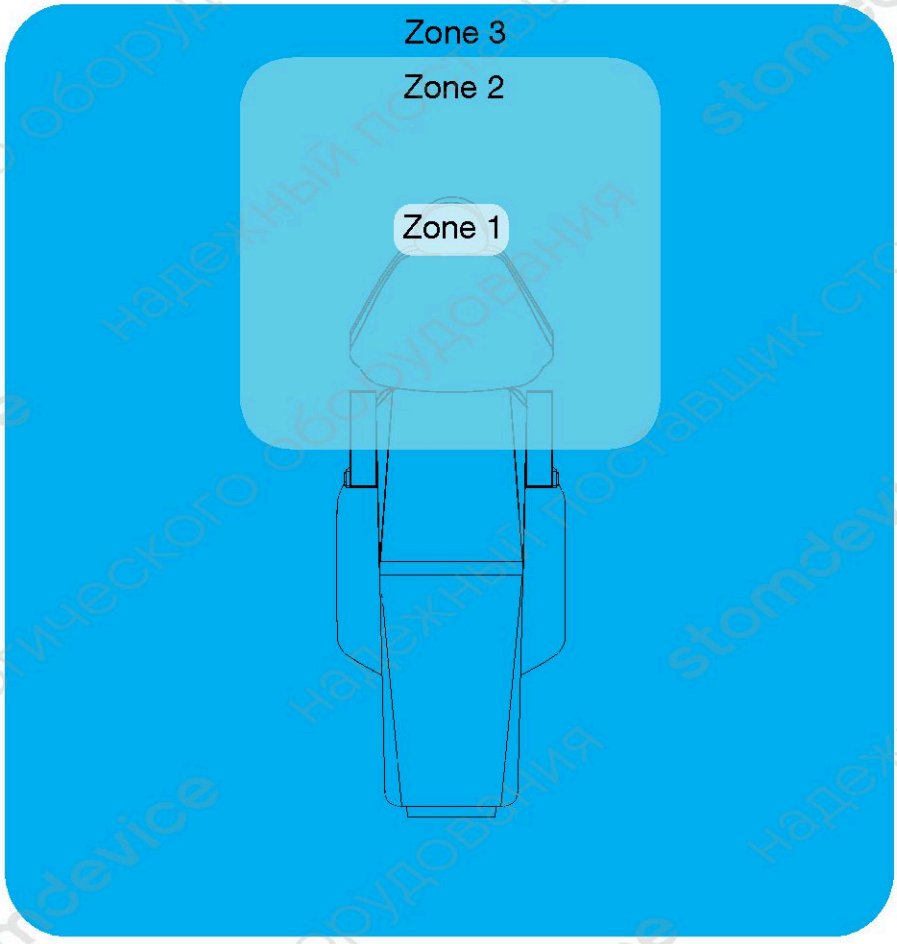

8. General information

Image of recommended light conditions for dentists.

- Zone 1 = 20 - 40 000 lux
- Zone 2 = 3 - 5000 lux
- Zone 3 = 500 - 1000 lux

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice


On-line support
http://www.d-tec.se/support

- Owner's manual
- Användarmanual
- Bedienungsanleitung
- Mode d'emploi

D-TEC LIGHTING SYSTEMS

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

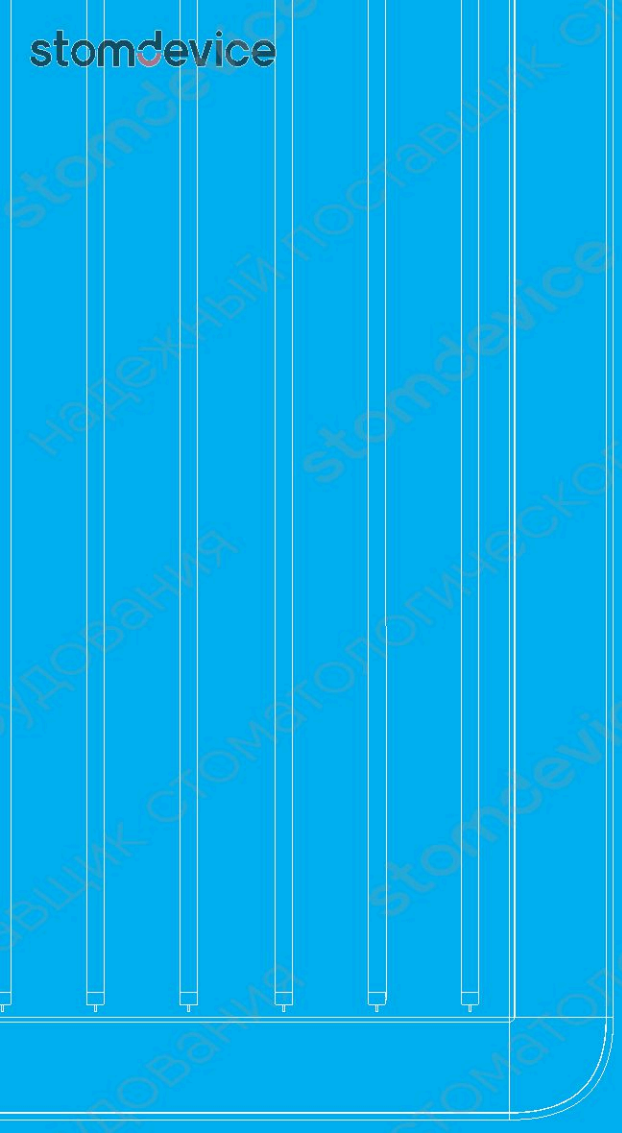

Facts: Denta/Dentaplus

- Environmentally friendly and energy-saving
- CDP (conical de-glaring prism)
- Option of indirect light and dimmer
- High intensity of illumination

  Denta: 4 000 lux/1,2 m

  Dentaplus: 280-5 800 lux/1,2 m
- Size 1 355 x 700 x 55 mm
- Weight 11 kg

D-TEC AB
Varavägen 12
SE-465 94 Nossebro
Tel +46 (0)31 969 302 Fax +46 (0)31 966 092
E-mail mailbox@d-tec.se
www.d-tec.se

D-TEC LIGHTING SYSTEMS

CE IM 18

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ