stomdevice

CE

発行日：2012 年 11 月 30 日制定

INSTRUCTION OF RUBBER DAM INSTRUMENTS

INSTRUMENTS;


KSK Rubber Dam Pun 132℃ Up to 132℃




KSK Rubber Dam Clamp Forceps 132℃ Up to 132℃



Rubber Dam Template Non - autoclavable




Rubber Dam Frame, Adult & Pedo 132℃ Up to 132℃




Dental Dams (6"x 6") 121℃ Dry heat is prohibited




Rubber Dam Clamp Boards 132℃ Up to 132℃

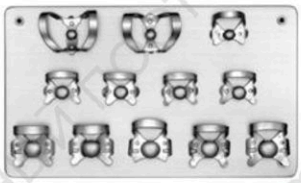

Rubber Dam Clamps 132℃ Up to 132℃

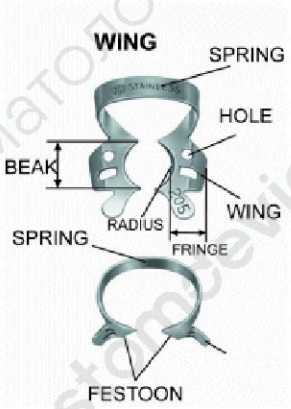

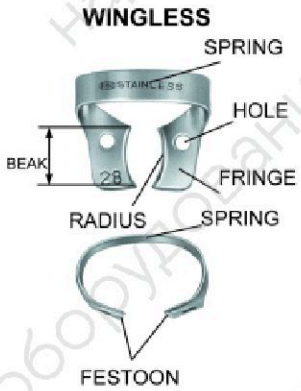

Molar:	15, 18, 24, 25, 26, 28, 30, 31,42,43 51, 138, 139, 200, 201, 202, 203, 204, 205, 3, W3, 4, 5, 56, 56A,7, 7A, 7B, 8, 8A, W8A, 10, 11, 12A, 13A, 14, 14A, 14AN
Bicuspid:	22, 27, 29, 206, 207, 208, 209, 1, 1A, 2, 2A, W2A, 0, 00
Labial:	210, 211, 212, 6, 9, 44, 90N
Deciduous:	P-1, P-2, 54, 55, 64, 65, 74, 75, 84, 85
Tiger:	1T, 1AT, 2T, 2AT, 14T, 56T, 9T
Others:	G-1, G-2


https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

INSTRUCTION;

1. Marking

The smooth side of Dental Dam is placed onto Rubber Dam Template, and teeth are marked according to Rubber Dam Template on the powdered side of Dental Dam.

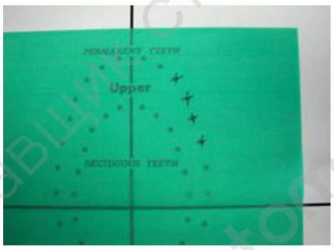

2. Punching


Marked teeth on Dental Dam are punched with KSK Rubber Dam Punch, in this time, correct holes should be chosen according to teeth





3. Positioning Clamp

A correct clamp suitable for a treated tooth is chosen with a reference to shape of clamps. The spring of the chosen clamp is pulled through the perforation of Dental Dam with KSK Rubber Dam Forceps. The clamp is positioned to the tooth smoothly.
Additional teeth are isolated in the usual way.

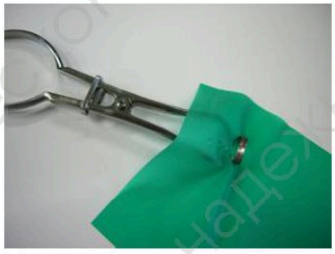



4. Fitting Frame

Dental Dam is fitted on Rubber Dam Fame accordingly.



Authorized representative

Four D Rubber Co Limited

Units 11-15 Slack Lane, Heanor Gate, Industrial Estate Hean or, Derbyshire, DE75 7GX

United Kingdom www.foudrubber.com

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ