
stomdevice

SINIUS

Treatment center care and cleaning plan

A continuously updated list of approved care, cleaning, and disinfecting agents can be downloaded from the Dentsply Sirona internet website under REF 59 70 905: www.sirona.com

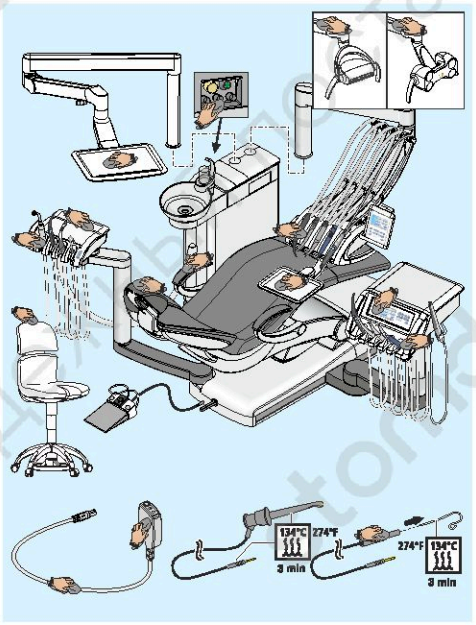


After each patient

Clean/disinfect surfaces

CAUTION! Use only care, cleaning, and disinfecting agents approved by Dentsply Sirona!

- Disinfect surfaces and upholstery
- Disinfect user interfaces
- Care, disinfection/sterilization of treatment instruments (see the operating instructions of the respective treatment instruments)
- Clean and disinfect/sterilize the components of the ApexLocator
- Disinfect instrument holders
- Disinfect handles
- Disinfect the tray
- Disinfect connectors for suction hose cleaning
- Maintain and clean the operating light (see LEDview or LEDview Plus operating instructions)

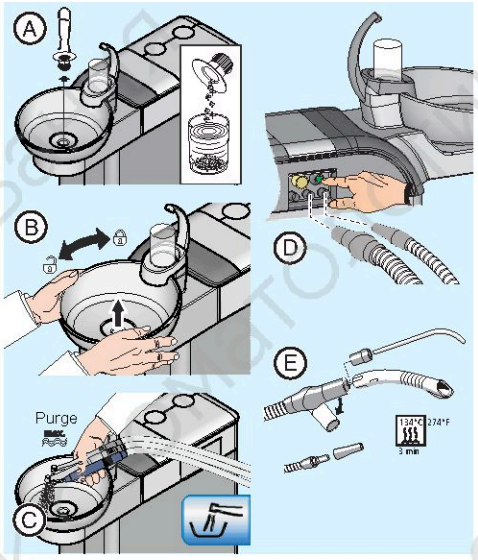

Clean/disinfect the water paths and suction system

CAUTION! Use only care, cleaning, and disinfecting agents approved by Dentsply Sirona!

A) Clean the gold trap

CAUTION! Dispose of amalgam residues in an environmentally correct manner!


B) Clean/disinfect the (removable) cuspidor bowl (special cleaning agent))

C) Purge the water lines of used dentist element instruments (Purge function)

D) Clean the suction hoses

E) Sterilize suction handpieces

To prevent reflux, please use the suction cannula with supplementary air intakes.

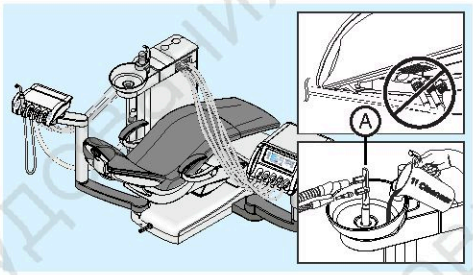


Daily

If the "Chemical hose cleaning" option is not available:

Disinfect the suction hoses using the cleaning adapters (A)


- daily at noon and
- and at the end of the work day.

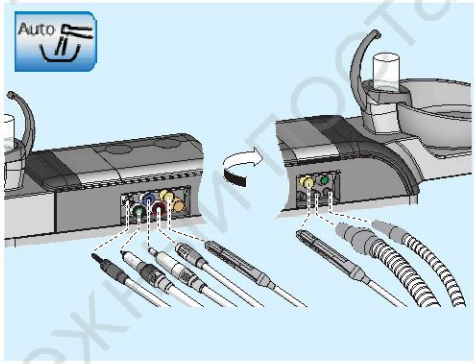

Automatically purge water lines (auto-purge function)

Insert the couplings into their corresponding adapters prior to the beginning of and at the end of the work day:

- white - high-speed handpiece
- green - BL motor
- blue - BL ISO E and BL ISO C motor
- red - Scaler
- yellow - SPRAYVIT, water on right button
- orange - SPRAYVIT, water on left button
- Suction hoses

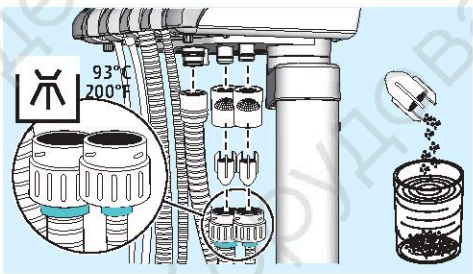


Clean the filters in the suction hoses

Collect amalgam residues in a closed container with water.

CAUTION! Dispose of amalgam residues in an environmentally correct manner!

Disinfect suction hoses


Suction hoses that can be thermally disinfected are marked turquoise.

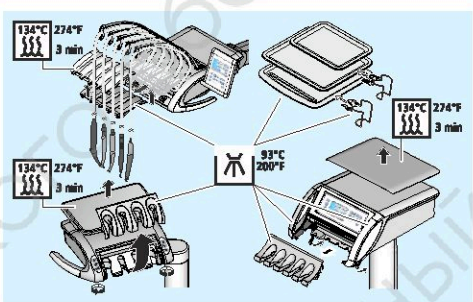

Thermally disinfect the instrument racks, tray, and cup holder

The silicone mats can be sterilized.

Weekly

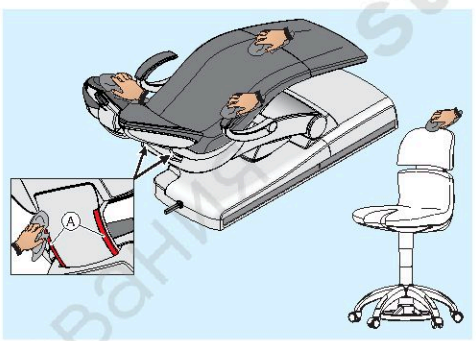


Clean and care for upholstery

CAUTION! Use only cleaning and care agents for upholstery approved by Dentsply Sirona!

Follow the instructions for use of the cleaning and care agents exactly.


Prevent agent FD360 from contacting chrome-plated surfaces.

Cleaning the bottom surface of the mount (A) for the backrest component

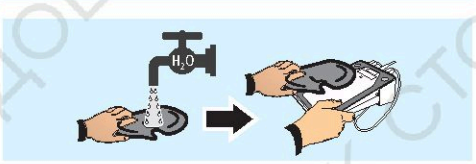

Clean the foot switch


Clean the underside of the foot control with a moist cloth.

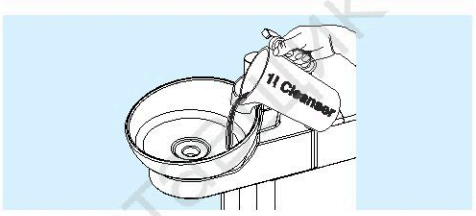


If the "Chemical hose cleaning" option is not available:

Clean drainage lines

The cleaning agents used for chemical cleaning of the hoses and of the suction system are identical (see REF 59 70 905).

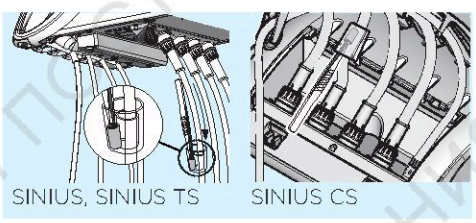


Change the cotton wool roll on the turbine hose

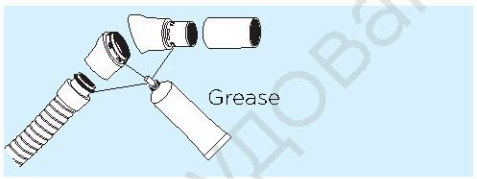

Lubricating suction handpieces

Separate suction handpieces and grease the O-rings after thermal disinfection or sterilization as well as once a week.

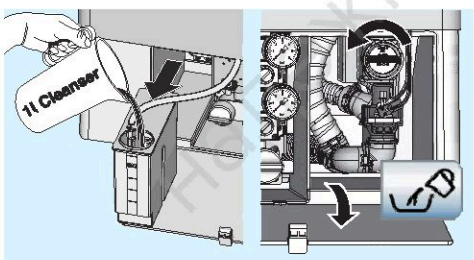


Monthly or as required

Refilling the cleaning agent tank

"chem" appears on the user interface: Refill the cleaning agent as soon as possible for chemical suction hose cleaning (optional).

Clean the filter insert of the standard wet suction

On the Start screen, press the "Extract residual water" button before removing the filter for cleaning.

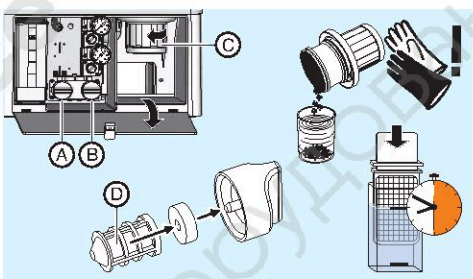


Change filter (D) for water (A) and air (B)

Empty the sediment tank (C) (optional)

Wear protective gloves when emptying the sediment tank!

Microbiological water test


- At regular intervals according to results and
- after periods of disuse > 1 week.

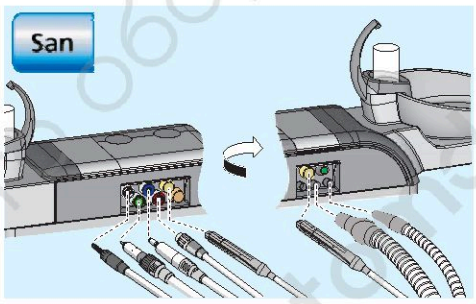

Sanitize the treatment center

For reduction of the biofilm within the fresh water carrying systems of the treatment center

- white - turbine
- green - BL motor
- blue - BL ISO E and BL ISO C motor
- red - Scaler
- yellow or orange - SPRAYVIT
- Suction hoses

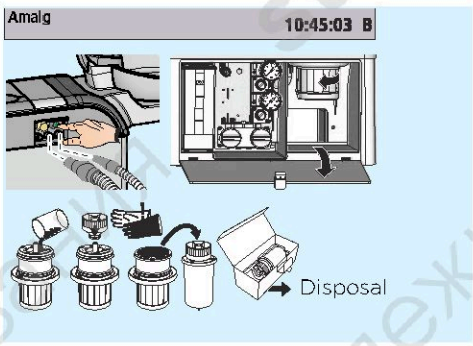

Replace amalgam rotor

IMPORTANT! The rotor must be replaced after 12 months at the latest!

1. "Amalg" appears on the user interface. Conduct disinfection.
2. Only with the unit switched on: remove amalgam rotor.
3. Fill in collected amalgam residues, close amalgam rotor.
4. Remove amalgam rotor from lower part and dispose of in an environmentally correct manner.

For more details, refer to the operating instructions.
The national requirements and recommendations for hygiene and disinfection must be observed (e.g. RKI, ADA, CDC etc).

THE DENTAL SOLUTIONS COMPANY™

Subject to technical changes and errors. Print no. D3561.104.01.09.02 Order no. 63 37 336 03.2017 Change no. 123 221

Dentsply Sirona

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ