
stomdevice

PLANMECA

# PLANMECA OLO DENTAL STOOL

## User's and installation guide

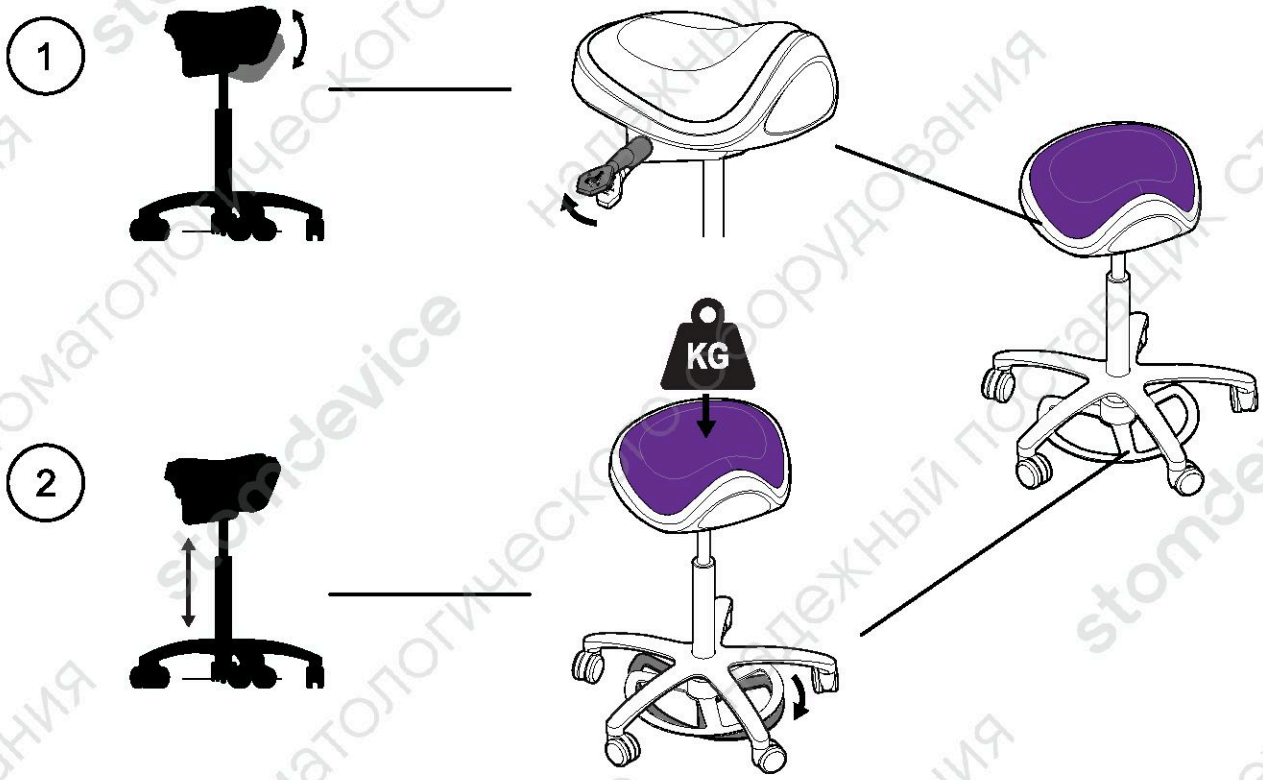



| | |
|---|---|
| 1. Seat angle | Pull and hold the lever upwards to unlock the seat and adjust the seat angle. Release the lever to lock the seat in the desired position.<br>Caution! Take care when tilting the chair forward so that you do not fall off the chair. |
| 2. Seat height | While putting weight on the seat, press and hold down the ring and adjust the seat to the required height. Release the ring to lock the position.<br>Note: You can rotate the ring (without pressing it) to adjust its position. |

Publication number 10040351 version 2
Copyright Planmeca
Released 20 April 2017

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

## Dimensions

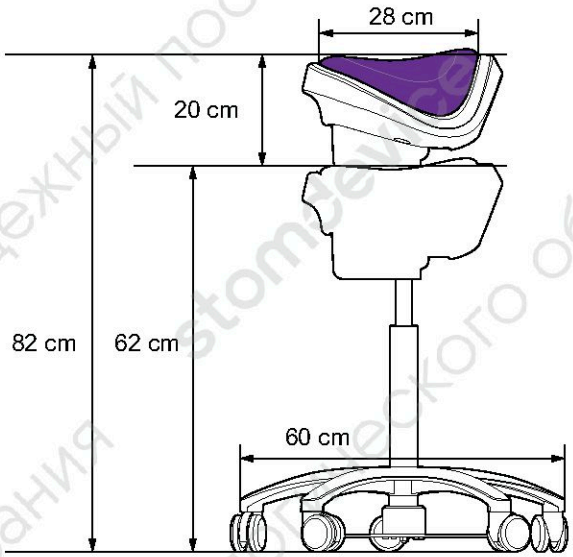


| | |
|---|---|
| Lowest seat height | 62 cm (24.4″)<br>(from floor to top edge of stool) |
| Highest seat height | 82 cm (32.3″)<br>(from floor to top edge of stool) |
| Range of adjustment of seat height | 20 cm (7.9″) |
| Seat depth | 28 cm (11″) |
| Seat width | 35 cm (13.8″) |
| Seat inclination | -4° - 10° |
| Weight | 10 kg |
| Free rotating caster wheels | ∅ 6.5 cm (2.6″) |
| Stool base | ∅ 60 cm (23.6″) |

## Cleaning

A mild soap and water solution can be used to wipe off stains and spills from the upholstery. Let the upholstery air dry.

For disinfecting the upholstery, we recommend Dürr FD 312 or a similar product.


Wipe all other parts clean periodically with Planmeca approved surface disinfectant (Dürr FD 333 / FD 322 or Orbis).

## Maintenance

If the dental stool is in need of maintenance, contact your local Planmeca dealer.

## Installing seat cushion

Place the seat cushion on the seat and attach it to the seat with two screws from the underside of the seat as shown in the picture below.

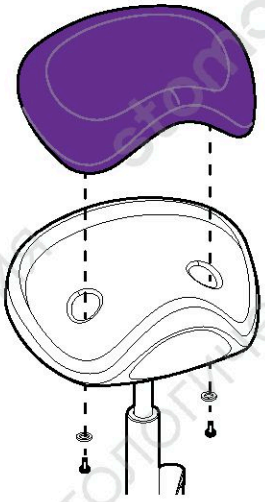



https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ