stomdevice

Planmeca Sovereign® Classic

Quick guide

Patient chair control

Control panel

Touch screen is unlocked. Press to lock. Touch screen is locked. Press and hold to unlock.

Backrest down
as long as pressed
(manual)



Backrest up
as long as pressed
(manual)



Chair down
as long as pressed
(manual)




Chair up
as long as pressed
(manual)




Chair to autoposition



View which foot control action drives chair to rinsing position

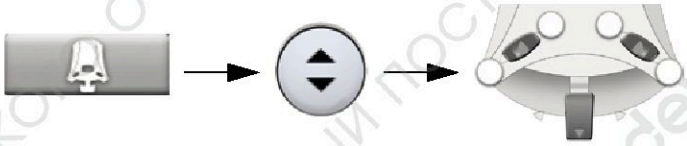

Foot control

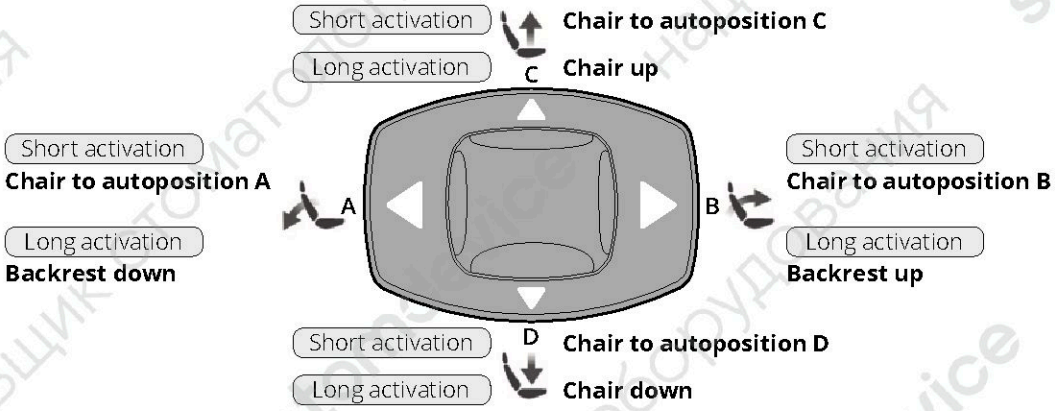


https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

Dental unit control

Control panel

Touch screen is unlocked. Press to lock. Touch screen is locked. Press and hold to unlock.

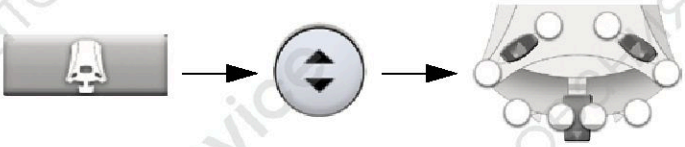Cup fill	Short activation	
Cup fill as long as pressed (manual)	Long activation	
Bowl rinse	Short activation	
Bowl rinse as long as pressed (manual)	Long activation	
Door open / assistant call function for preprogrammed time	Short activation	
Door open / assistant call function as long as pressed (manual)	Long activation	
Operating light On ► Off	Short activation	
Intensity of operating light (manual)	Long activation	
Operating light's composite mode On ► Off	Short activation	
Intensity of operating light in composite mode (manual)	Long activation	
Start required timer	 → Select timer number	
Maintenance procedure	 → Select procedure	
View programmed foot control functions		

Foot control

Functions can be programmed.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

Instrument control

Control panel

Touch screen is unlocked. Press to lock. Touch screen is locked. Press and hold to unlock.

Automatic chip blow
On ► Off

Fibre optic light
On ► Off

Water & air ► Air ► No spray

Scaler
Spray 1 ► Spray 2 ► No spray

Scaler
Change operation mode

Turbine
Power reduction On ► Off

Turbine
Quickstart On ► Off

Micromotor
Reverse rotation On ► Off

Micromotor
RPM limit On ► Off


Micromotor
Preset selection

Micromotor
Torque limit On ► Off

Micromotor
Toggle drive mode when torque limit On

Auto stop | Auto reverse | Auto forward

View programmed foot control functions

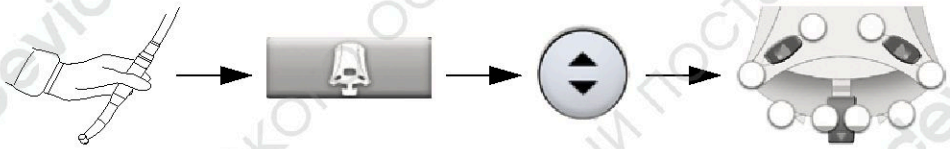

Foot control

Functions can be programmed.

stomdevice

Programming

Control panel

Touch screen is unlocked. Press to lock. Touch screen is locked. Press and hold to unlock.

Patient chair autoposition settings

The function is enabled. The function is disabled.




Move chair to required position → Switch operating light On/Off → Start programming → Press chair positions button → Select autoposition → Accept new autoposition

Unit settings

The function is enabled. The function is disabled.

Most programming follows this simple sequence:

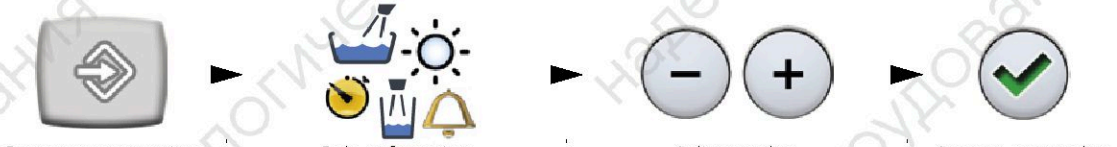

Start programming → Select function → Adjust value → Accept new value

Instrument settings

The function is enabled. The function is disabled.

Most programming follows this simple sequence:




Activate instrument → Start programming → Select function → Adjust value → Accept new value

Flexy button functions



Start programming → Press Flexy holder button → Press button next to Flexy figure → Select function → Accept new function

Foot control functions

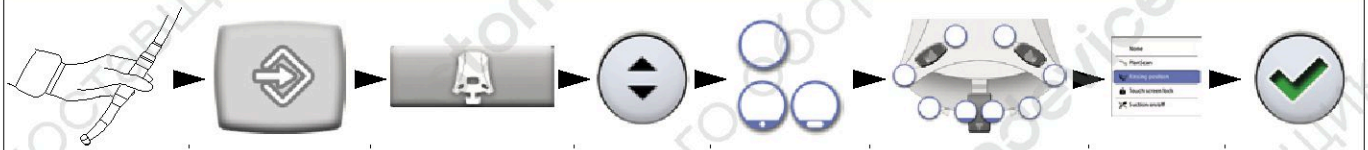

Activate instrument (optional) → Start programming → Press foot control button → Select group → Select push mode → Press button next to desired action → Select function → Accept new function

Time and date settings

The function is enabled. The function is disabled.



Start programming → Select time and date → Select function → Select format → Adjust value → Accept new value

10036725_4/11.2017/en

For detailed instructions, please see the user's manual. Copyright Planmeca. Rights for changes reserved.

www.planmeca.com

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ