
stomdevice

WATER DEMINERALIZER

PURE 500

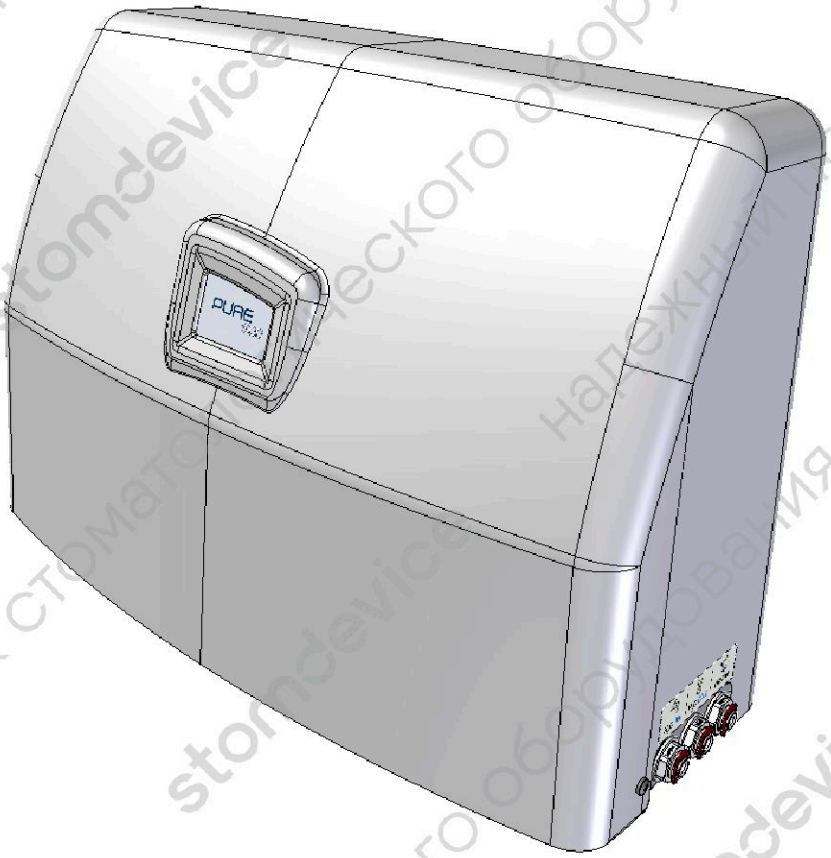

OPERATING MANUAL

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

REVISIONS

The following table lists subsequent editions/revisions of the manual.
The "Description" field brief explains the subject of the latest revision.

Code	Rev.	Date	Description
97050638	3	12-2017	Text adaptation

TABLE OF CONTENTS

ENGLISH (TRANSLATION FROM THE ORIGINAL IN ITALIAN)
INTRODUCTION 3
INTENDED USE 3
PURPOSE OF THE MANUAL 4
GENERAL WARNINGS 4
CONTENTS OF THE PACKAGE 5
DIMENSIONS AND WEIGHT 5
PRODUCT HANDLING AND STORAGE 5
DESCRIPTION OF THE CONTENTS 6
PRODUCT PRESENTATION 7
MAIN PERFORMANCES 7
VIEWS (WITH DIMENSIONS) 7
INSTALLATION 9
GENERAL PRECAUTIONS 9
SAFETY PRECAUTIONS 9
INSTALLING THE OSMOTIC MEMBRANE CARTRIDGE 11
CONNECTING PURE 500 TO AUTOCLAVES 16
CONNECTING TO THE WATER MAINS 18
OPERATION 21
FIRST STARTING 21
PRECAUTIONS TO PREVENT WATER STAGNATION 21
APPENDIX A - TECHNICAL CHARACTERISTICS 22
SUMMARY TABLE 22
APPENDIX C - MANTEINANCE 23
GENERALS 23
APPENDIX C - MANTEINANCE 29
WATER BLOCK® SAFETY VALVE MAINTENANCE 29
PERIODIC CHECK OF THE ANTI-BACKFLOW DEVICES 29
DISPOSAL AT END-OF-LIFE 29
APPENDIX D - TROUBLESHOOTING 30
APPENDIX Z - CUSTOMER SUPPORT 31

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

INTRODUCTION

Dear Customer,

Thank you for choosing a product. We hope that you will find it completely satisfactory.
This manual describes all procedures for the correct installation and use of the equipment.
Should you have any questions or suggestions concerning this product or our support, do not hesitate to contact us.

Note, warning and danger symbols used through the manual

	**NOTE** PAY SPECIAL ATTENTION; NOTES FOR PROPER INSTALLATION AND MAINTENANCE PROCEDURES AND USE METHODS.

	**WARNING!** THIS SYMBOL INDICATES A POTENTIAL DANGER OF INJURY. FOLLOW THE PRO-CEDURES DESCRIBED IN THE MANUAL TO AVOID INJURING THE USER AND/O.

Symbols on equipment

	Appliance equipped with water anti-backflow device in accordance with the EN 1717 standards..
	Equipment in accordance with applicable directives.
	Waste disposal in accordance with Directive 2012/19/UE.
	Consult the user manual.

INTENDED USE

The appliance is intended for professional use and only for the purpose for which it was designed, that is, demineralization of drinking water and its subsequent use to feed steam sterilizers.

ENGLISH

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

NOTE

THE INFORMATION IN THIS MANUAL IS SUBJECT TO CHANGE WITHOUT NOTICE. M.O.COM. SRL SHALL NOT BE RESPONSIBLE FOR DIRECT, INDIRECT, ACCIDENTAL OR CONSEQUENTIAL DAMAGE OR OTHER DAMAGES RELATED TO THE SUPPLY/ USE OF THIS INFORMATION.

THIS DOCUMENT MAY NOT BE REPRODUCED, ADAPTED OR TRANSLATED, IN WHOLE OR IN PART, WITHOUT THE PRIOR, WRITTEN AUTHORIZATION OF M.O.COM. SRL

THE ORIGINAL MANUAL IN ITALIAN SHALL BE CONSIDERED THE VALID INTERPRETATION OF THESE INSTRUCTIONS.

PURPOSE OF THE MANUAL

The manual purpose is to provide instructions for:
- general knowledge of the product;
- correct installation;
- its safe and efficient use.

More the appendix includes:
- the technical features of the product;
- maintenance operations;
- troubleshooting and solutions;
- other documentation.

GENERAL WARNINGS

The product must always be used according to the procedures included in this manual and never for purposes other than the ones indicated.

WARNING!

THE USER IS RESPONSIBLE FOR ALL LEGAL REQUIREMENTS RELATED TO THE INSTALLATION AND USE OF THIS PRODUCT. THE MANUFACTURER WILL NOT BE RESPONSIBLE FOR ANY BREAKAGE, MALFUNCTIONS, PROPERTY DAMAGE OR INJURY IN THE EVENT THAT THE PRODUCT IS NOT INSTALLED OR USED CORRECTLY.

Please observe the following precautions in order to avoid injury or property damage; in particular:
- use **ONLY** recommended cleaning detergents;
- **do not** pour water or other liquids or inflammable products on the equipment;
- **do not** use the equipment in the presence of gas or explosive or inflammable vapors;
- **do not** remove any label or nameplate from the device; request new ones, if necessary;
- use **only original replacement parts;**
- **do not** occlude or kink the water tubes leading to and from the appliance;
- **do not** feed sterilizing autoclaves with water produced from exhausted filters.

WARNING!

THE FAILURE TO OBSERVE THE ABOVE, RELEASES THE MANUFACTURER FROM ALL LIABILITY.

WARNING

THE WATER PRODUCED BY PURE 500 CANNOT BE USED FOR FOOD PURPOSES.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ


CONTENTS OF THE PACKAGE

NOTE
CHECK THE INTEGRITY OF THE PACKAGE UPON RECEIPT.

Once the package is opened, check that:
- the supply matches the specifications of the order (see the accompanying document);
- that there is no obvious product damage.

DIMENSIONS AND WEIGHT

Size and weight	Pure 500
Height	mm 490
Width	mm 295
Depth	mm 555
Overall weight	kg 7,6

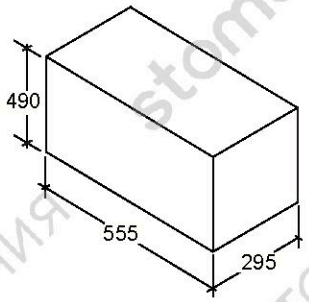

NOTE
IN THE CASE OF A WRONG PRODUCT, MISSING PARTS OR ANY TYPE OF DAMAGE, IMMEDIATELY PROVIDE A DETAILED DESCRIPTION TO THE RESELLER AND THE TRANSPORTER THAT MADE THE DELIVERY.

PRODUCT HANDLING AND STORAGE


The product must be handled following the instructions given on the packaging.

NOTE
KEEP THE ORIGINAL PACKAGING AND USE IT EACH TIME THE APPLIANCE IS TRANSPORTED. USING DIFFERENT PACKAGING MIGHT CAUSE DAMAGE TO THE PRODUCT DURING TRANSPORT.

WARNING!
FULLY DRAIN OUT THE WATER CONTAINED IN THE DEMINERALIZER BEFORE TRANSPORT.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

DESCRIPTION OF THE CONTENTS

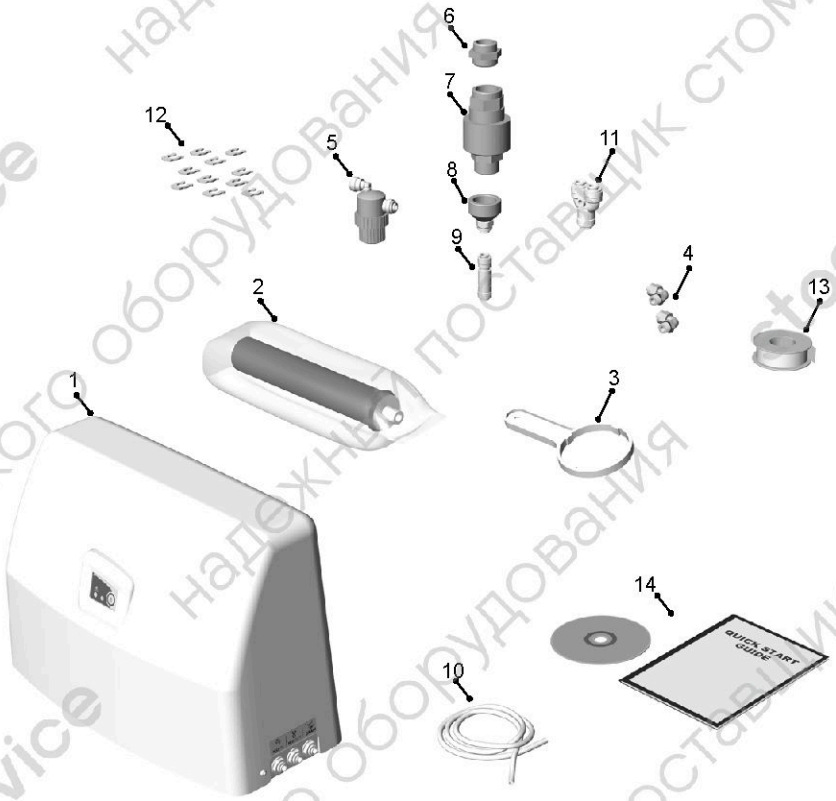

1) Demineralizer body;
2) osmotic membrane cartridge;
3) wrench for fitting/removing the osmotic membrane vessel;
4) 2 PIPU unions for 1/4" Ø tube
5) net minifilter;
6) 1/2" female - 3/4" male reducer;
7) safety valve (WATER BLOCK®) with filter and adjustment wrench;
8) 3/4" female straight terminal for 1/4"Ø tube;
9) non-return valve EA;
10) filling tube (6 m, 1/4" Ø);
11) intermediate quick-coupling;
12) 11 1/4" tube holding clips;
13) teflon tape;
14) warranty certificate + declaration of conformity + quick start guide + CD-ROM.

NOTE
THE CUSTOMER MUST KEEP THE WARRANTY CERTIFICATE TOGETHER WITH THE RECEIPT.

ENGLISH

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

PRODUCT PRESENTATION

Pure 500 is a reverse osmosis demineralizer, a natural addition to the range of steam sterilizers.
It has an elegant and compact design that combines ease of use and high reliability.
Pure 500 is hence an interesting option for users that require professional devices with an excellent quality/price/performance ratio.


MAIN PERFORMANCES


Pure 500 has been designed to demineralize mains drinking water for subsequent automatic feeding into steam sterilizers.

The solid structure in plastic and steel and the ergonomic and essential shape allows maintaining a high level of hygiene, reduced weight and dimensions and excellent stability during use.
All this with the aim of offering a product suited to the daily needs in the medical field.

VIEWS (WITH DIMENSIONS)

FRONT

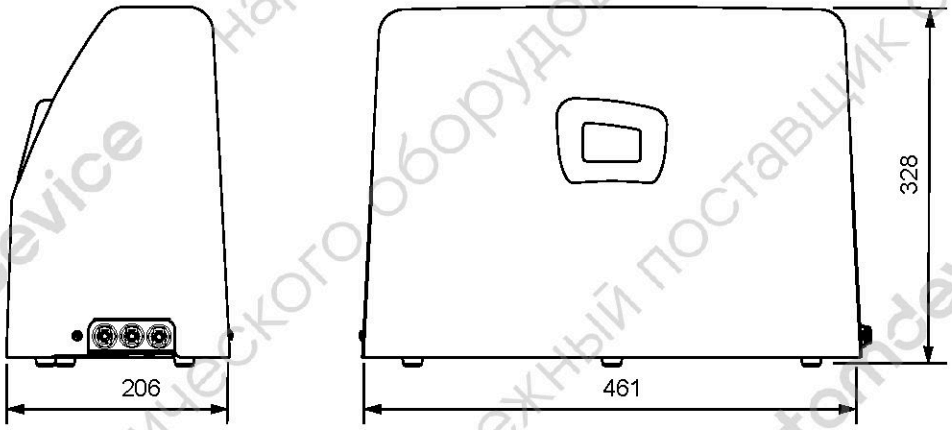


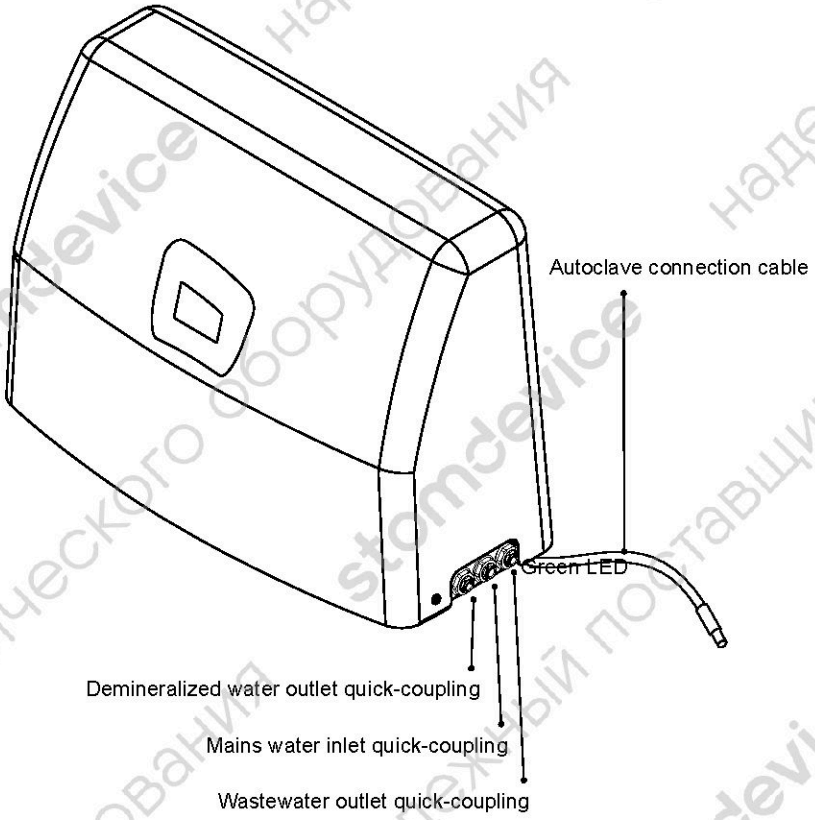

ENGLISH


https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

BOTTOM

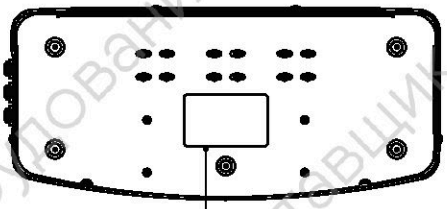


Serial number label

REAR

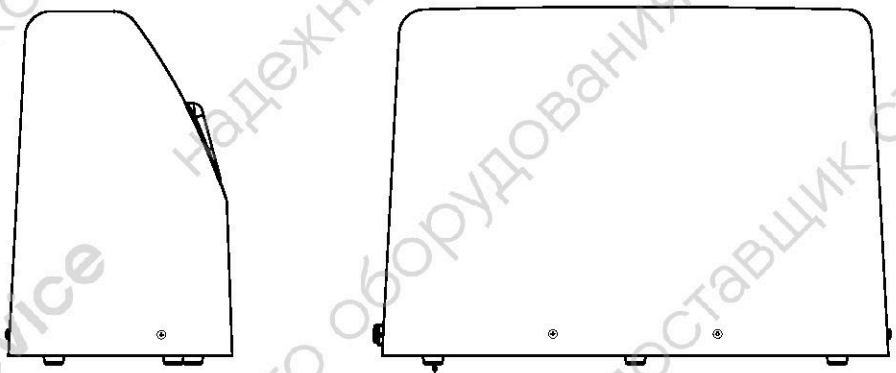

Support feet

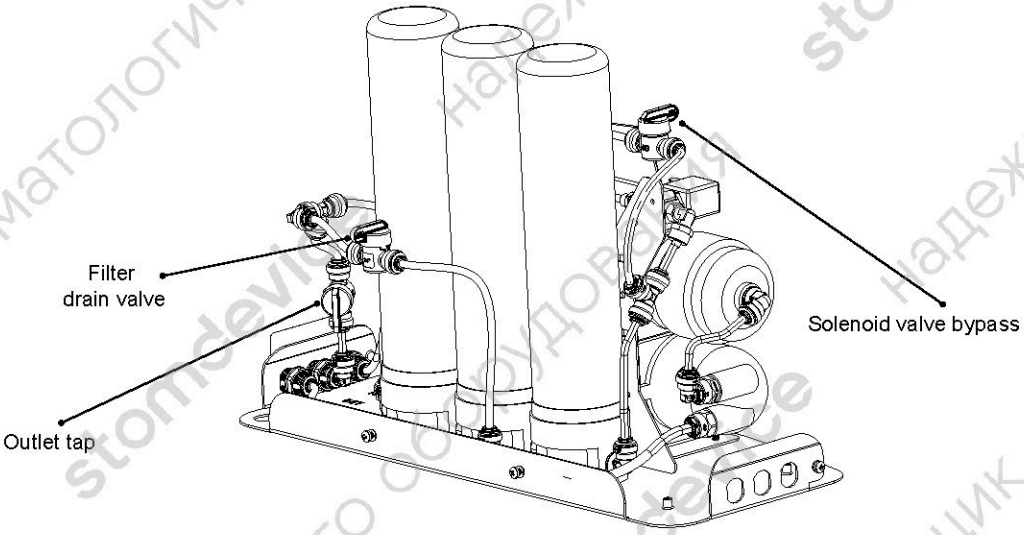

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

INSTALLATION

For good functioning of the demineralizer, the first essential operation to be carried out is proper installation, in order to prevent malfunctions or damage to the appliance. Please **scrupulously** observe the warnings given further on in this section.

☞	**NOTE** THE TECHNICAL SERVICE (SEE APPENDIX Z) IS AT YOUR DISPOSAL, TO CLEAR ANY QUESTIONS OR PROVIDE FURTHER INFORMATION.

GENERAL PRECAUTIONS

- Install Pure 500 on autoclaves using the accessories provided with the demineralizer;
- do not install in humid or poorly ventilated environments;
- do not install in environments where there are flammable and/or explosive gases or vapours;
- install the appliance in such a way that the water tubes are not kinked or crushed.

SAFETY PRECAUTIONS

Described below are the instructions to follow in the event of contact with the ionic exchange resins contained in the Pure 500 demineralizer cartridges.

RISKS ON CONTACT	
Contact with the eyes.	Irritating to eyes (R36).
Contact with the skin.	Slightly irritating to skin.
FIRST AID	
Contact with the eyes.	Immediately and abundantly wash with water and remove all particles.
Contact with the skin.	Take off contaminated clothes.
	Remove the particles and wash the affected area with water.
MEASURES IN THE EVENT OF ACCIDENTAL DISPERSION	
Precautions for persons.	Keep away from persons.
	Pay attention on slippery floors to avoid dropping the appliance.
Decontamination methods.	Collect the product and transfer it to suitable plastic containers for recovery or disposal as indicated.
NOTES ON DISPOSAL	
The used product is non-hazardous special waste.	
The product must be disposed of in compliance with the local, regional or national regulations in force.	
The CER number for saturated or exhausted ionic exchange resins used to prepare drinking water or water for industrial use is: **190905**.	

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

Listed below are the actions to take in the event of contact with the activated carbon filter contained in Pure 500.

RISKS ON CONTACT	
Contact with the eyes.	Possible temporary irritation because of abrasive dust.
Contact with the skin.	Possible temporary irritation because of abrasive dust.
FIRST AID	
Contact with the eyes.	Do not rub the eyes.
	Immediately wash with plenty of running water holding the eyelids wide open for at least 15 minutes (to remove the dust).
	If necessary, seek medical advice.
Contact with the skin.	The product cannot be absorbed through the skin. It may cause dehydration or slight irritation because of abrasive dust.
	Immediately take off contaminated clothing and wash the skin with soap and water.
	In the case of dehydration symptoms, seek medical advice.
MEASURES IN THE EVENT OF ACCIDENTAL DISPERSION	
Precautions for persons.	Keep away from persons.
	Makes the floor slippery: be careful to avoid falling.
Decontamination methods.	Clean with mechanical means or a vacuum cleaner to prevent the formation of dust. Use appliances that do not generate electrical charges or sparks.
NOTES ON DISPOSAL	
In the case of a virgin product: dipose of at an authorised dumping ground.	
If the product is exhausted (having absorbed substances): use different disposal techniques depending on the nature of the substances absorbed and the national and local regulations in force. The CER number is: **190904**.	


https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

INSTALLING THE OSMOTIC MEMBRANE CARTRIDGE

Take the osmotic membrane cartridge and the vessel fitting/removing wrench out of the accessory kit:


A) Undo the screws (1) that secure the cover to the frame of the demineralizer using a cross-head screwdriver (not provided).

B) Lift the plastic cover (2) of the demineralizer and place it on a flat surface.

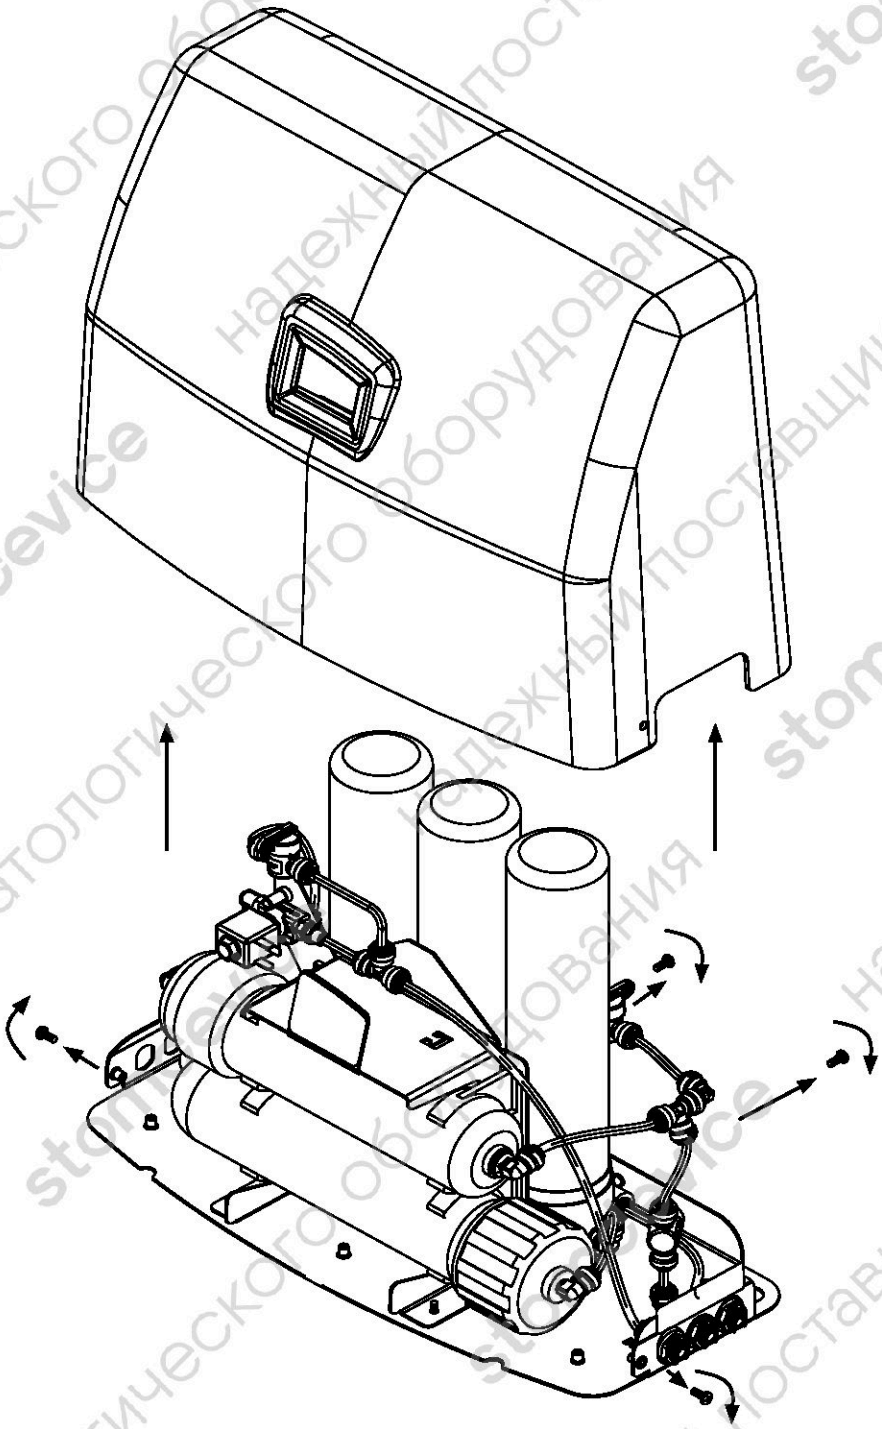


https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

C) Remove the safety clip (7) of the quick-coupling (8) on the head (4a) of the osmotic membrane vessel (4), then remove the tube (9) from the coupling.

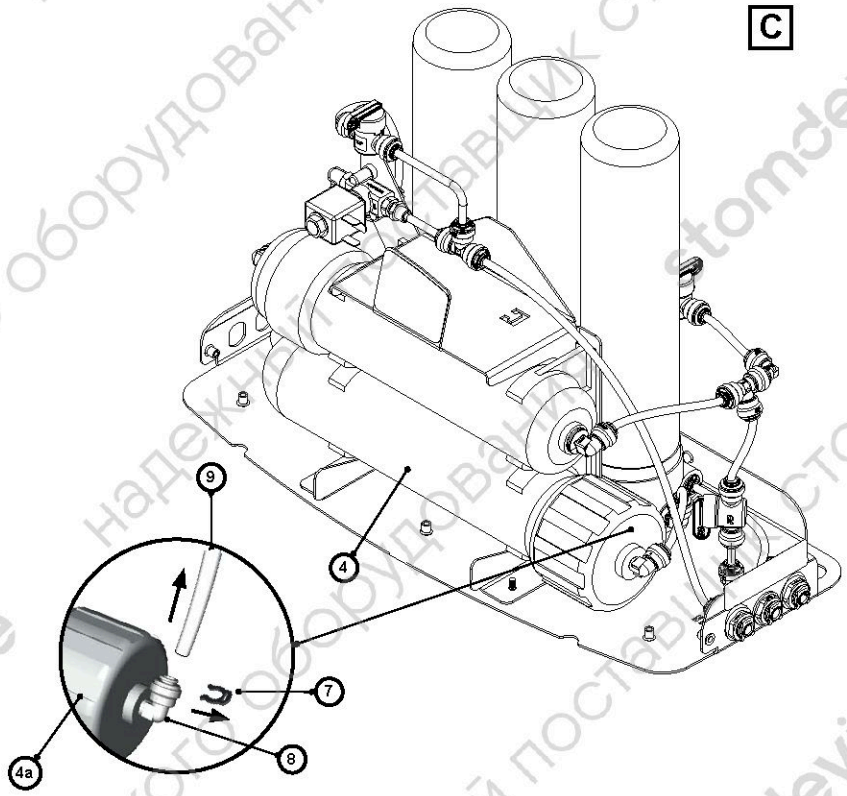


D) Using both hands, grip the membrane vessel (4) positioned horizontally in the front part of the demineralizer and remove it from the brackets (5) fitted on the Pure 500 frame.

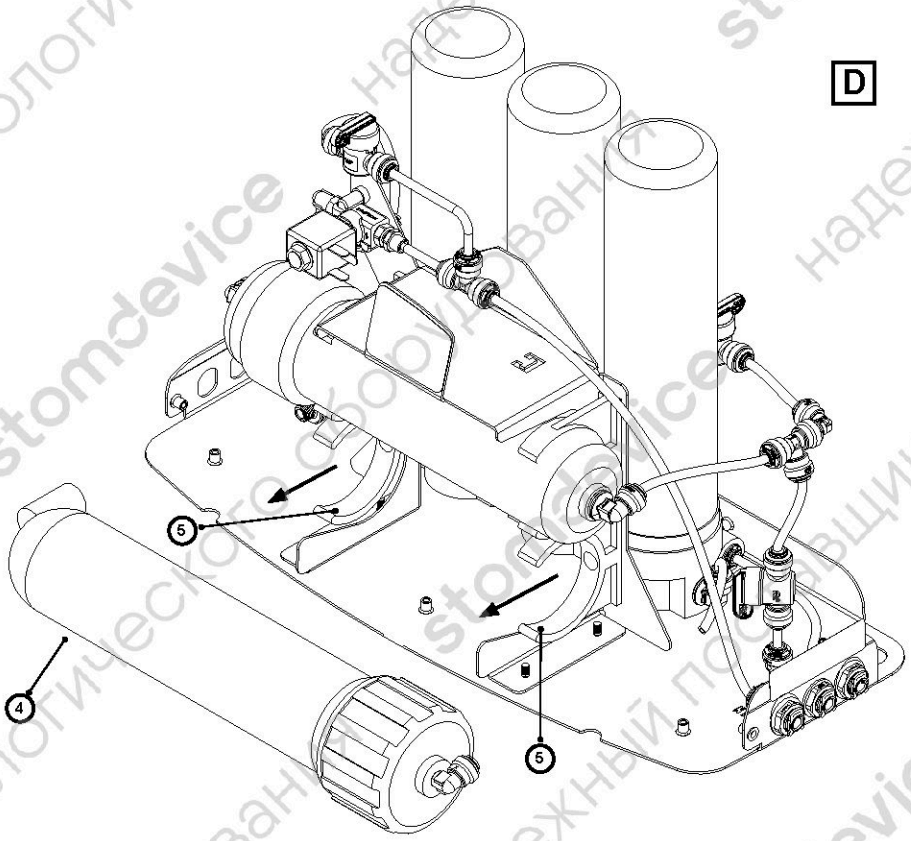

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ


E) Unscrew the head (4a) of the osmotic membrane vessel (4) using the wrench (10) contained in the accessory kit.

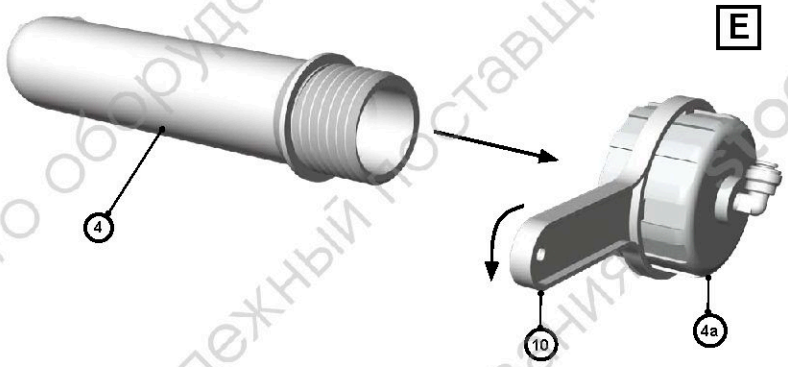

F) Remove the protective bag of the osmotic membrane cartridge (11).


G) Insert the osmotic membrane cartridge (11) in the osmotic membrane vessel (4).

H) Screw on the head (4a) of the osmotic membrane vessel (4) using the wrench (10).

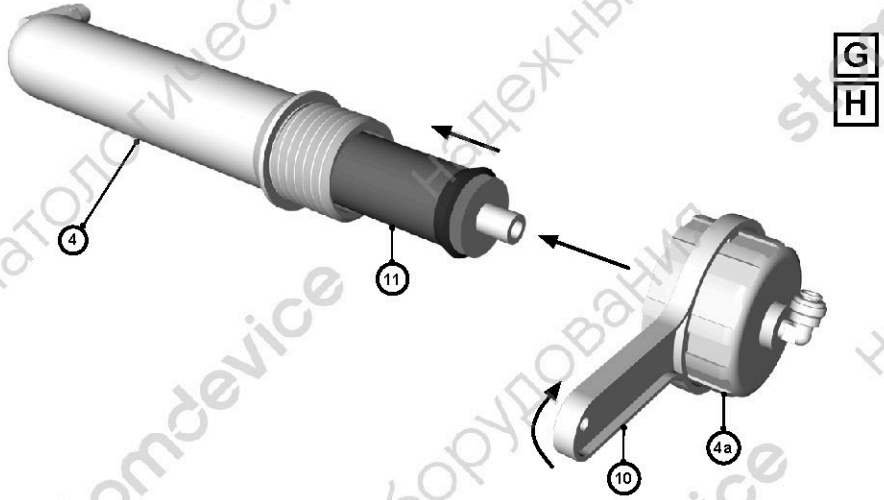


https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

I) Refit the osmotic membrane vessel (4) in the brackets on the frame.

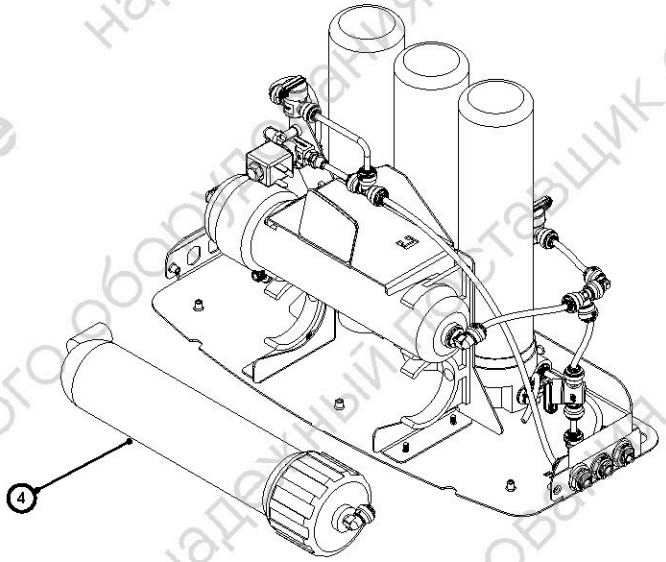


I

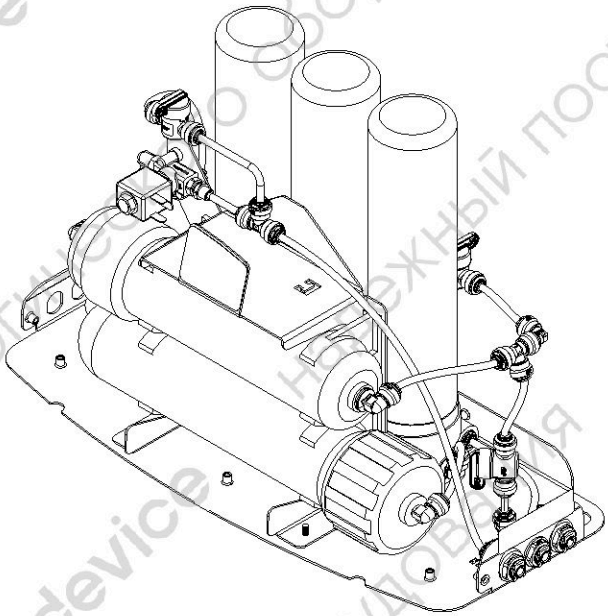

J

L) Insert the tube (9) in the quick-coupling (8) on the head (4A) of the osmotic membrane vessel (4), then fit the safety clip (7) on the coupling.

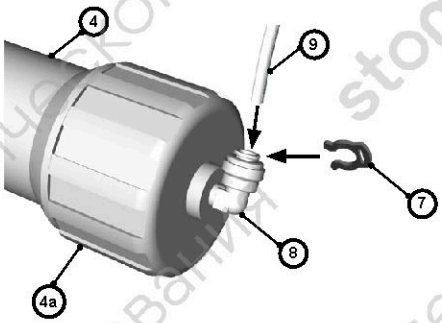


L

ENGLISH

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

M) Reposition the demineralizer cover (2) and fasten it to the frame with the screws (1)

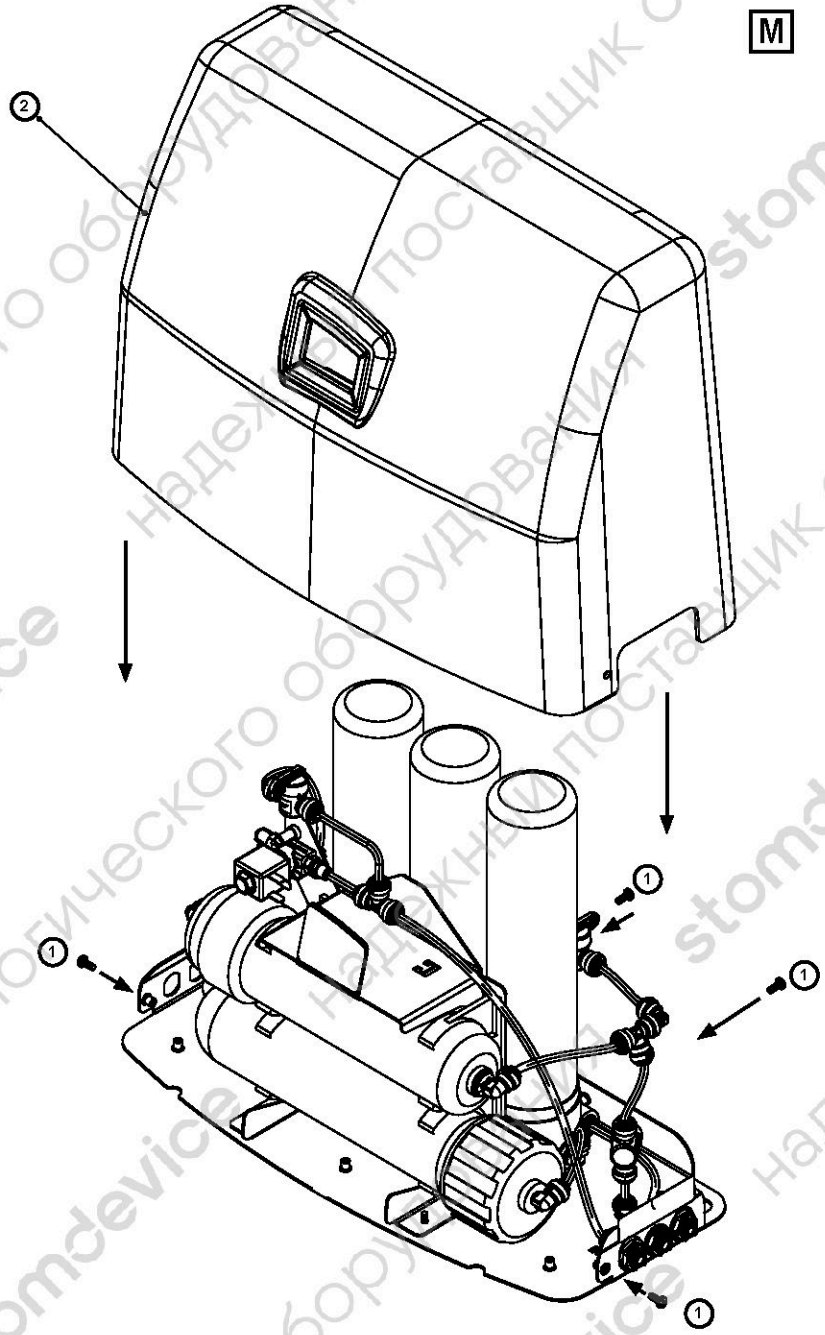

⚠	**WARNING** DURING INSTALLATION, PUT THE PLASTIC COVER BACK ON THE DEMINERALIZER **ONLY AFTER** HAVING CORRECTLY FOLLOWED THE INSTRUCTIONS FOR OPENING AND CLOSING THE TAPS ON THE PURE 500 BODY, INDICATED IN THE PROCEDURE "FIRST STARTING" (PAR. 5.1).


https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

CONNECTING PURE 500 TO AUTOCLAVES

Pure 500 must be installed on the right-hand side of the autoclaves using the devices that form part of the standard equipment of the demineralizer.

M) Take the following out of the accessory kit:
- the filling tube (3 m, 1/4" Ø)
- 1 spigot union for 1/4" Ø tube
- the net minifilter;
- 2 tube holding clips

N) Remove the tube holding clip and the cap on the rear of the autoclave adapted for automatic filling.

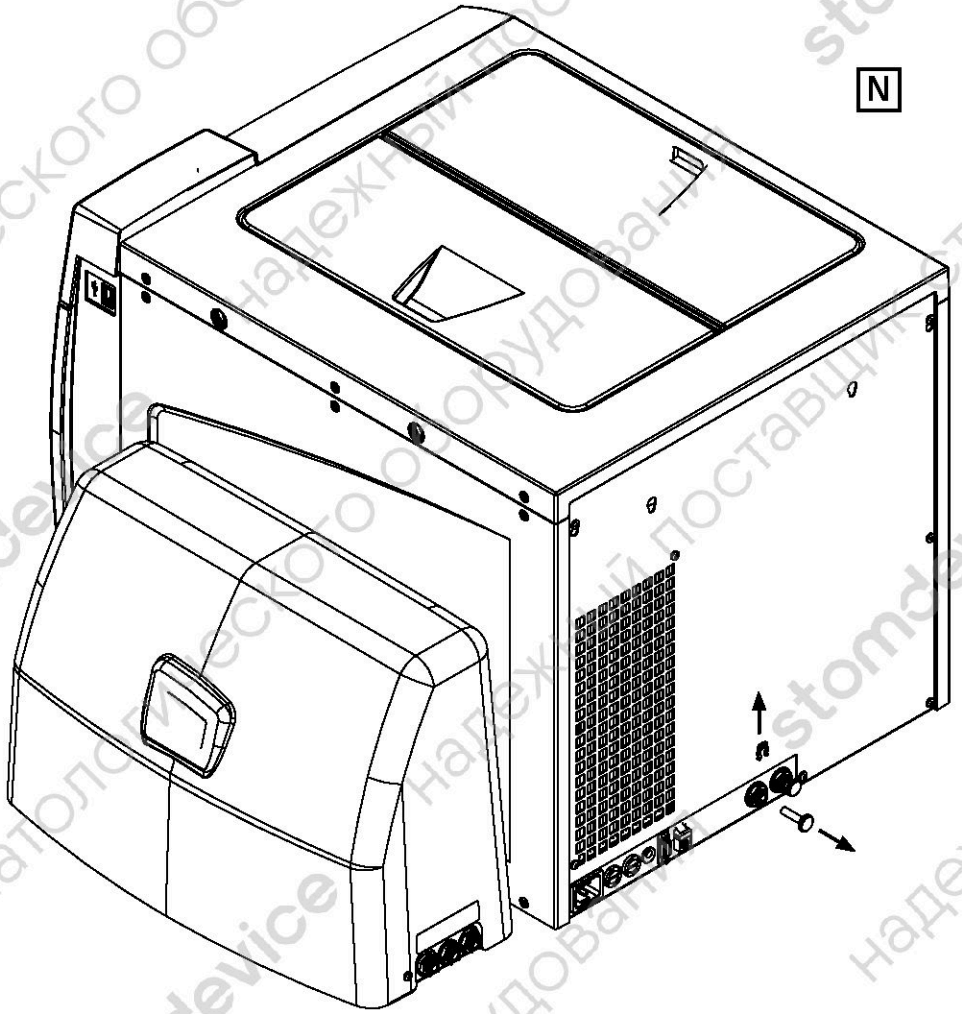

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ


O) Fit 1 spigot union for 1/4" tube (5) to the female union just freed (J) in the rear wall of the autoclave.

P) Take the tube provided and cut 2 pieces with the following lengths:
- tube (7) = 30 cm
- tube (8) = 20 cm

Q) Fasten one end of the tube (7) to the demineralized water outlet quick-coupling of Pure 500 and then fasten the other end to the minifilter inlet quick-coupling provided (10)..

R) Fasten the tube (8) to the minifilter outlet quick-coupling and then fasten the other end to the spigot union for 1/4" tube (5) previously fitted on the autoclave.

S) Fit the tube holding clips in the relative seats of the quick-couplings of the demineralizer (to prevent the tubes from accidentally slipping out).

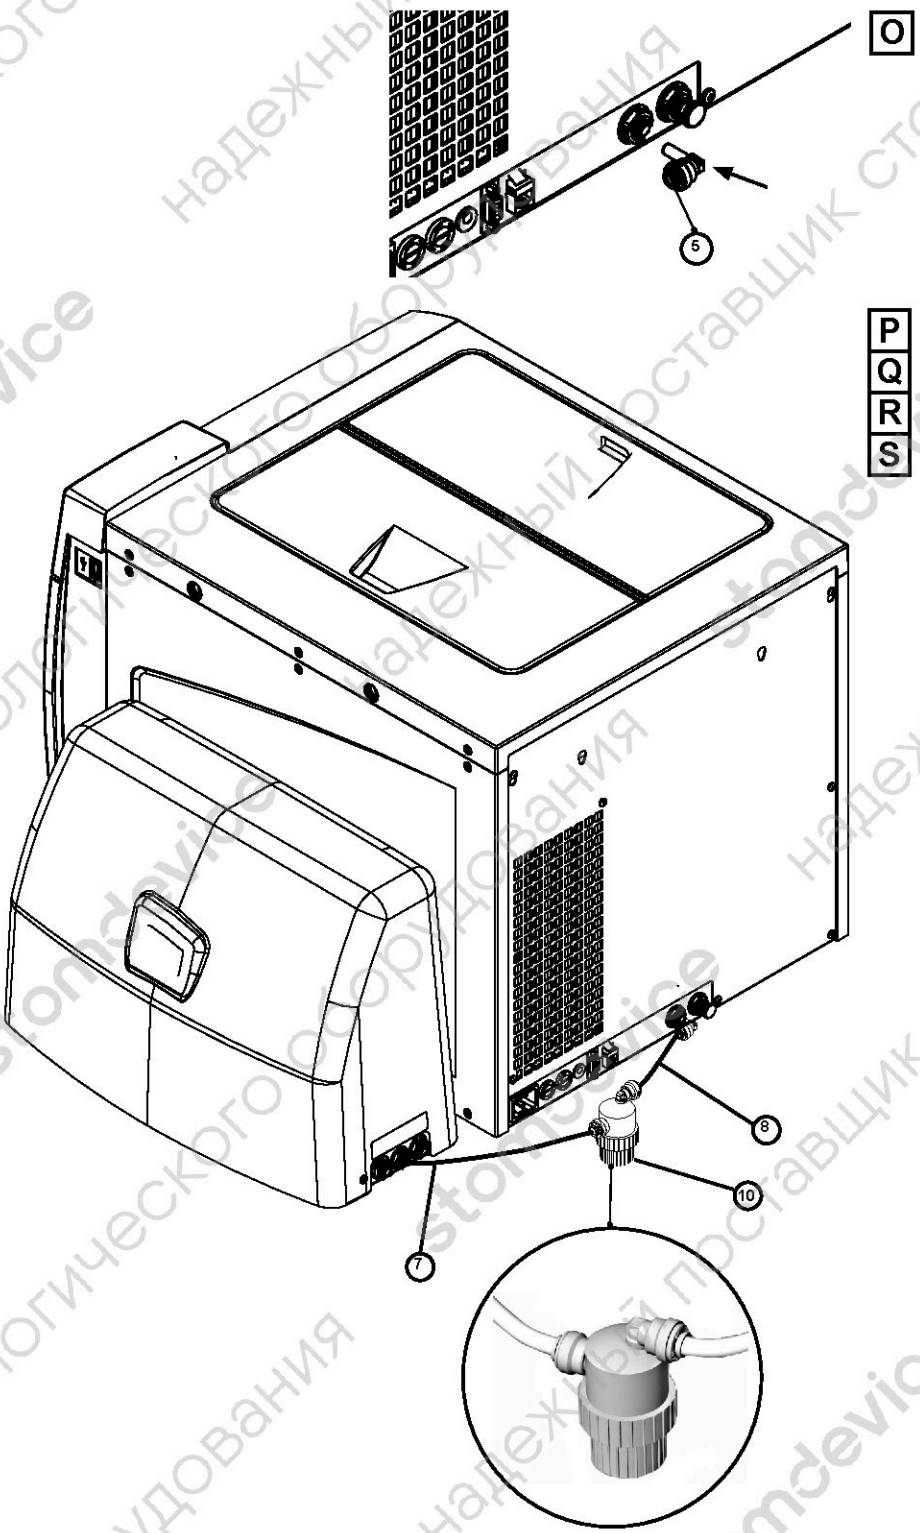

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

CONNECTING TO THE WATER MAINS

For Pure 500 to function it needs to be connected to a mains drinking water tap using the devices supplied standard with the demineralizer:

T) Take the following out of the accessory kit:
- the 1/2" female-3/4" male reducer;
- the safety valve (WATER BLOCK®);
- the 3/4" female terminal for 1/4" Ø tube;
- the non-return valve;
- the filling tube (6 m. 1/4" Ø);
- 1 1/8" male elbow union for 1/4" Ø tube;
- the intermediate quick-coupling;
- 7 tube holding clips.

U) Fit the 1/2" female-3/4" male (25) reducer between the utility tap and the WATER BLOCK® valve (26) only when the tap has a 1/2" male coupling. Use Teflon tape to ensure a tight seal.
If the tap has a 3/4" male coupling, the WATER BLOCK® valve can be screwed on directly (put the reducer (25) back in the accessory kit).
N.B. The WATER BLOCK® valve must be positioned vertically as indicated in the instruction leaflet in the relative package.

V_1) Screw the straight terminal (27) onto the 3/4" male thread on the WATER BLOCK® valve outlet.


V_2) Take the tube provided and cut 3 pieces with the following lengths:
- tube (28) = 5 cm
- tube (29) = 200 cm
- tube (30) = 100 cm

V_3) Fasten the tube (16) to the outlet quick-coupling of the straight terminal (15).

V_4) Take the non-return valve (18) and fit it on the free end of the tube (16).

V_5) Fasten one end of the tube (17) to the outlet quick-coupling of the non-return valve (18)

V_6) Fit the tube holding clips in the relative seats of the quick-couplings fitted (to prevent the tubes from accidentally slipping out).

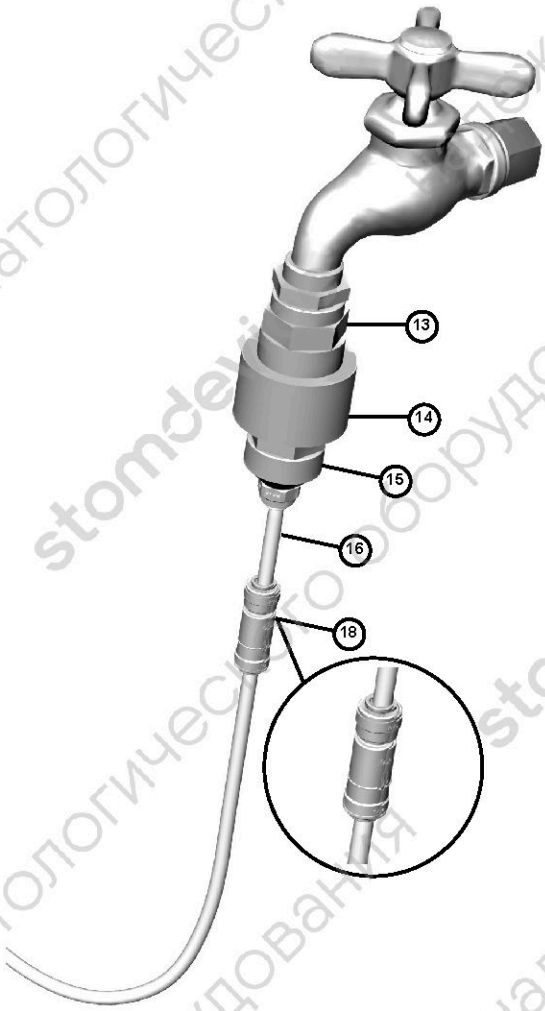


U
V_1
V_2
V_3
V_4
V_5
V_6

ENGLISH

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

W) Fasten the other free end of the tube (17) to the Pure 500 (19) inlet.

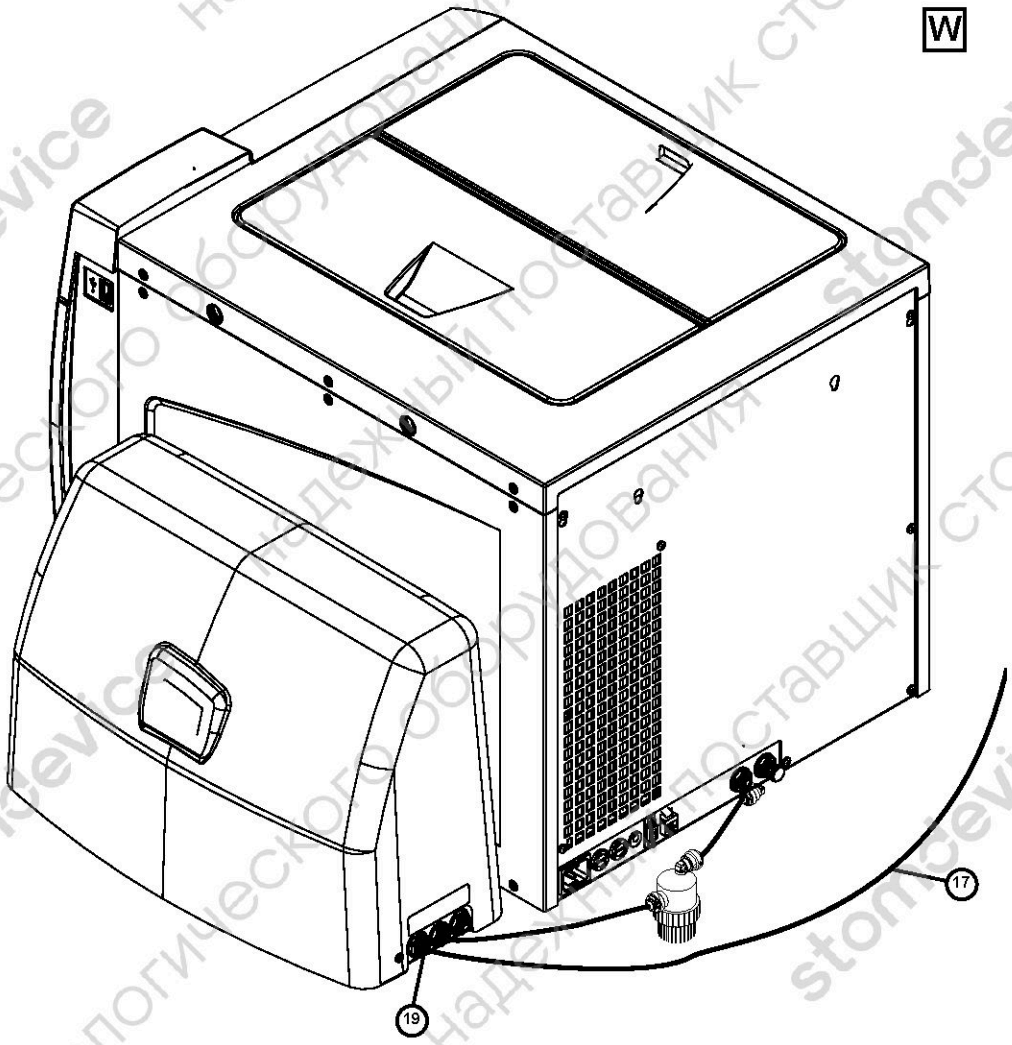

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

Y_1) Fasten one end of the tube (30) to the wastewater outlet quick-coupling (32) of Pure 500, then fasten the other end to the intermediate quick-coupling (33).

Y_2) Take a spigot union for 1/4" tube (35) and, after removing the clip and cap, insert it in the free outlet union on the rear wall of the autoclave.


Y_3) Take the drainage tube provided with the autoclave and cut off a piece 100 cm long (34).

Y_4) Fasten one end of the tube (34) to the spigot union for 1/4" tube (35) already fitted on the autoclave, then fasten the other end to the intermediate quick-coupling (33).

Y_5) Take the remaining concentrate drainage tube (36) provided with the autoclave and insert one end in the outlet of the intermediate coupling (33).


⚠	**WARNING** TO CONNECT THE FREE END OF THE TUBE (36) TO THE CENTRAL DRAIN POINT OF THE USER, SEE THE DEDICATED PARAGRAPH IN THE AUTOCLAVE USER MANUAL.

Y_6) Fit the tube holding clips in the relative seats of the quick-couplings fitted (to prevent the tubes from accidentally slipping out).

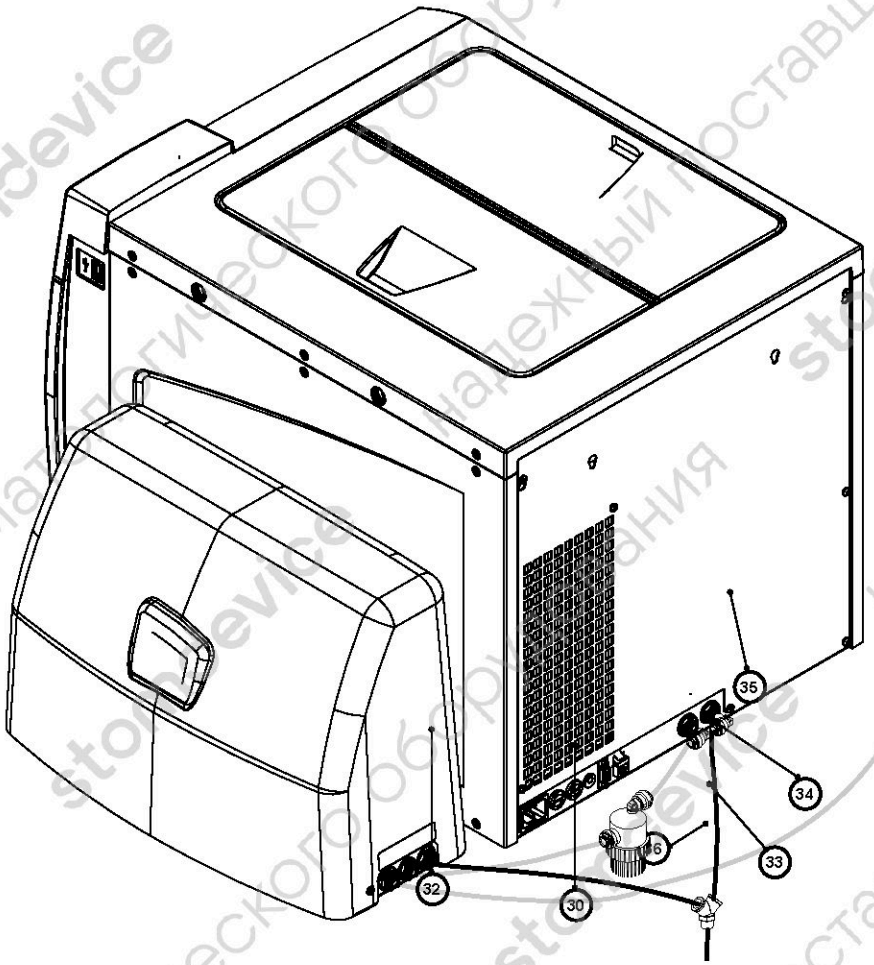

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

Z) Connect the plug (38).

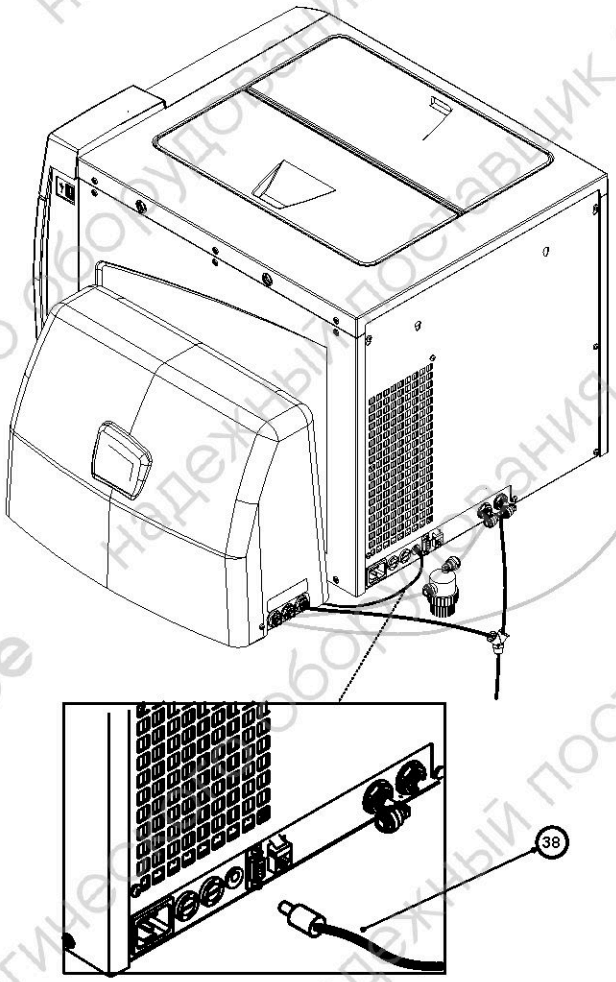

OPERATION

FIRST STARTING

In order to start using the Pure 500 demineralizer, all the installation phases must have been correctly carried out:

A) fitting of the osmotic membrane cartridge (par. 4.3.);
B) connection of the autoclaves (par. 4.4.);
C) the water mains connected (par. 4.5.);
D) the mains drinking water tap opened;
E) the drinking water inlet tap on the demineralizer body opened;
F) closing of the filter drain valve on the demineralizer body;
G) the batteries inserted (par. 4.6.);
H) turning on the autoclave.

⚠	**WARNING** WHEN THE DEMINERALIZER IS TURNED ON OR CONNECTED, THE AUTOCLAVE DETECTS THE PRESENCE OF AN AUTOMATIC FILLING SYSTEM AND ASKS YOU TO SET WHICH SYSTEM HAS BEEN CONNECTED.

⚠	**WARNING!** ALWAYS CLOSE THE MAINS DRINKING WATER TAP AT THE END OF THE WORKING DAY AND BEFORE PROLONGED PERIODS OF INACTIVITY OF THE DEMINERALIZER.

PRECAUTIONS TO PREVENT WATER STAGNATION

Drain out all the water from the demineralizer if it is not to be used for long periods of time.

⚠	**WARNING!** FAILING TO FULLY DRAIN OUT PURE 500 LEADS TO DEGRADATION OF THE WATER QUALITY AND PROLIFERATION OF BACTERIA AS A RESULT OF WATER STAGNATING IN THE DEMINERALIZER TUBES AND IN THE STERILIZER TANKS.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

APPENDIX A - TECHNICAL CHARACTERISTICS

SUMMARY TABLE

Model	PURE 500
Manufacturer	CEFLA s.c. Headquarters Via Selice Provinciale 23/A – 40026 Imola (BO) IT
Operating temperature	+5°C ÷ +30°C
Storage temperature	+5°C ÷ +30°C
Dimensions (L x D x H)	461 x 206 x 328 mm
Weight (without cartridges)	5,6 kg
Use	Indoors
Power supply voltage	3 VDC supplied by two 1.5V AA batteries*
Incoming water	Tap drinking water
Outgoing water quality	Conductivity < 15µS/cm**
Water mains minimum and maximum pressure	2-5 bar
Water mains minimum and maximum temperature	+5°C ÷ +40°C
Demineralized water production	approx. 800 litres***

* Value suggested by the EN 13060 standards.

** The quantity of water produced by the filter cartridges depends on the quality and the hardness of the mains water.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

APPENDIX C - MANTEINANCE

GENERALS

The equipment does not need any special care; it is only recommended that the user cleans it periodically.

In all cases carefully follow the procedure detailed below.

IIn case of replacement of equipment components, request and use ONLY ORIGINAL SPARE PARTS.

EXTERIOR CLEANING

Clean the equipment externally with a clean cloth dampened with water and neuter detergent.

	NOTE - DO NOT USE PRODUCTS CONTAINING ISOPROPYL ALCOHOL (2-PROPANOL, ISO-PROPANOL); - DO NOT USE PRODUCTS THAT CONTAIN SODIUM HYPOCHLORITE (BLEACH); - DO NOT USE CLEANERS THAT CONTAIN PHENOL.


Perfectly dry the surfaces and remove any remaining resistant residue.

Always keep in mind the following general warnings:

- do not submit the unit to direct water jets, under pressure or sprinkling. Any infiltration on the internal electrical components could irremediably damage its operation.
- Do not use abrasive sponges, metal brushes (or other aggressive materials) or products for cleaning of metal, both solid and liquid.

FILTER CARTRIDGE REPLACEMENT

Upon activation of the alarms warning that the conductivity values in the demineralized water produced are higher than the permitted limit (15µS/cm), the filter cartridges need to be replaced:




A) Turn off the autoclave.



B) Drain out the autoclave filling tank (see the sterilizer user manual).

C) Remove the plastic cover of Pure 500:


- undo the screws that secure it to the frame of the demineralizer using a cross-head screwdriver (not provided);
- lift the cover and position it on a flat surface.

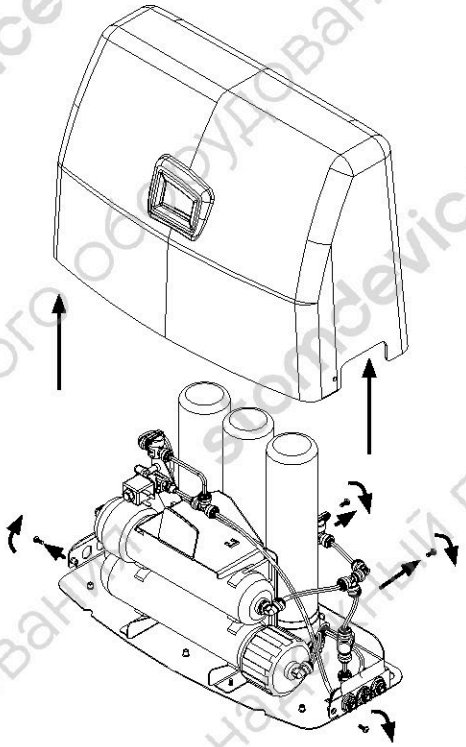

ENGLISH


https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

D) Open the drain and close the outlet.

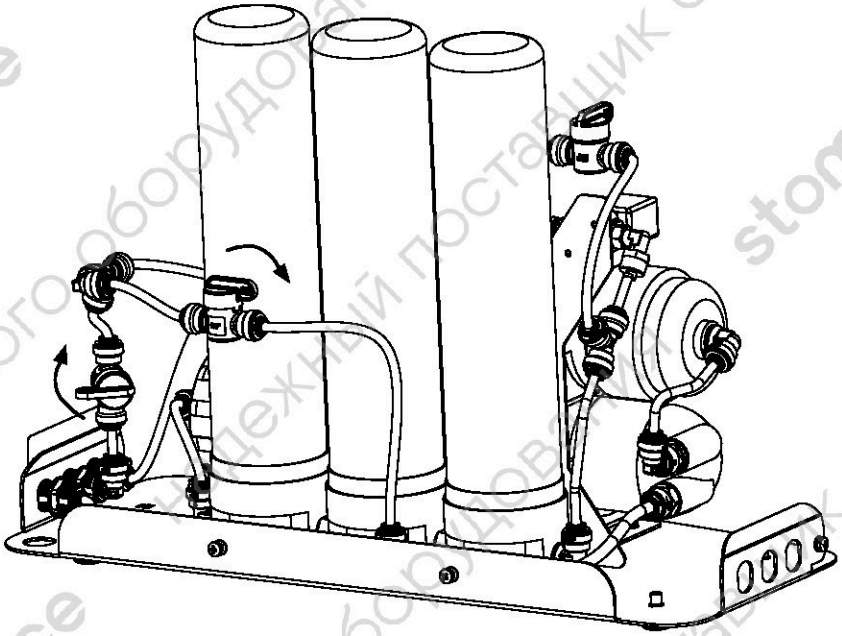


E) Remove the three vertical filter cartridges (SEDIMENT + ACTIVATED CARBON + IONIC EXCHANGE RESIN) from the relative quick-coupling heads positioned on the frame of the demineralizer.

- Dry off any water that has spilled out with a cloth;
- dispose of the three quick-coupling filter cartridges in compliance with the regulations in force.

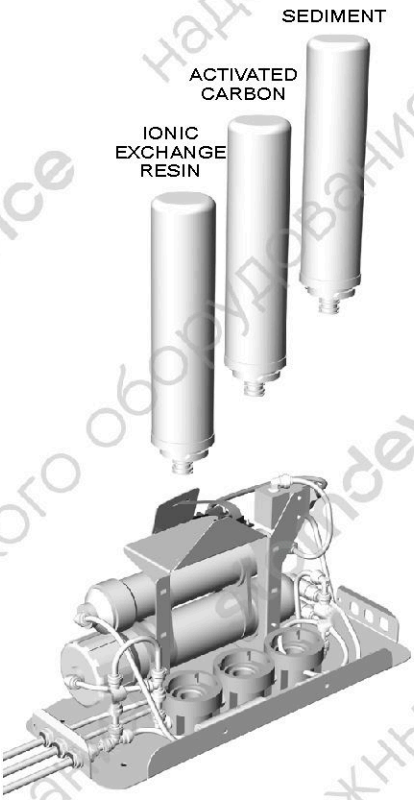

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

F) Take the new set of quick-coupling filter cartridges (SEDIMENT + ACTIVATED CARBON + IONIC EXCHANGE RESIN) and screw them into the respective heads on the frame of the demineralizer.

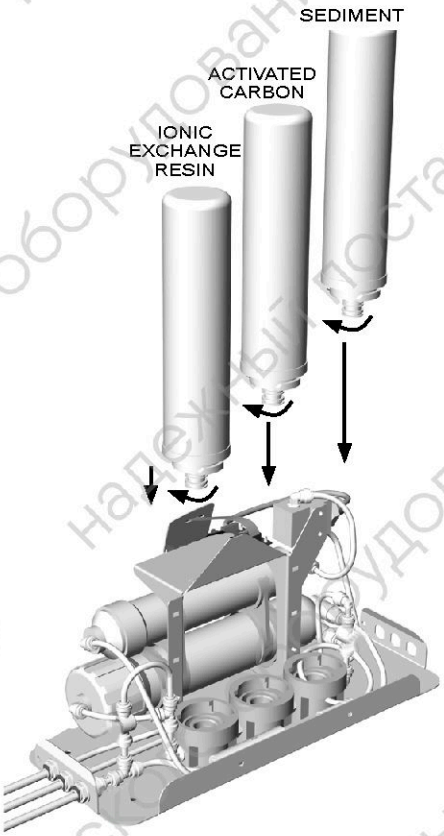

G) OSMOTIC MEMBRANE CARTRIDGE REPLACEMENT


Take the vessel fitting/removing wrench out of the accessory kit and remove the exhausted cartridge found inside the vessel.

- Drain out the water that has remained in the vessel and then fit the new cartridge as described in Paragraph 4.3. “INSTALLING THE OSMOTIC MEMBRANE CARTRIDGE”;
- dry off any water that has spilled from the vessel and the exhausted cartridge;
- dispose of the exhausted osmotic membrane cartridge in compliance with the regulations in force.


https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

H) REPLACING THE INLINE RESIN CARTRIDGE

- Release the cartridge from the clips that join it to the osmotic membrane cartridge vessel.
- Remove the tubes that connect the resin cartridge to the hydraulic circuit of the demineralizer.
- Unscrew the quick-couplings fitted on the two heads of the resin cartridge.

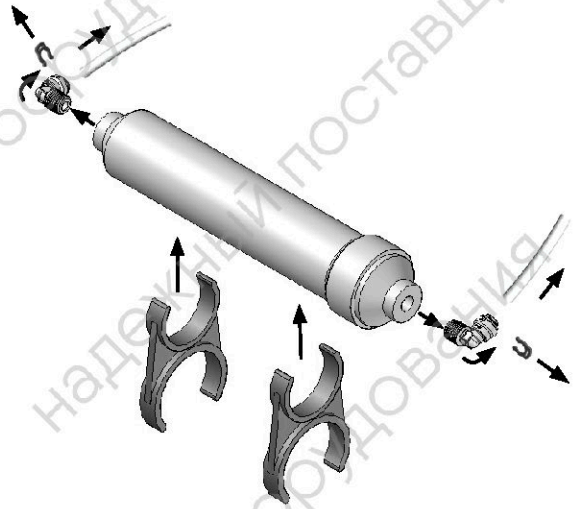


- Dry off any water that has spilled out with a cloth.
- Dispose of the resin cartridge in compliance with the regulations in force.
- Remove the inline resin cartridge wrapping.
- Screw the quick-couplings previously removed (point H) onto the heads of the new cartridge. Use the Teflon tape to secure their fitting.
- Refit the tubes that connect the resin cartridge to the hydraulic circuit of the demineralizer.
- Refit the resin cartridge in the clips fitted on the osmotic membrane cartridge vessel.

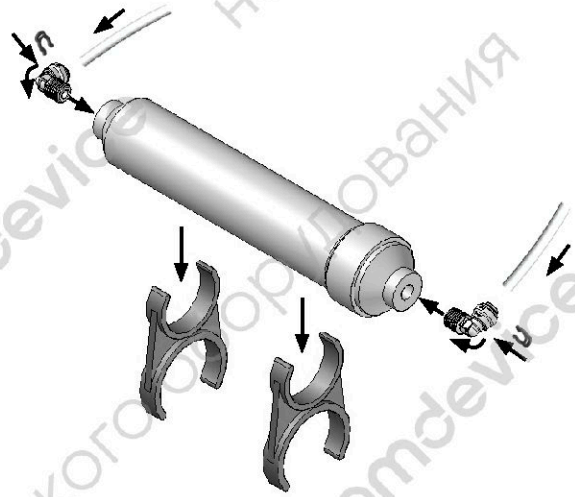


https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ


I) When you have finished changing the cartridges, open the tap on the solenoid valve and drain water for about 15 minutes to clean the cartridges.

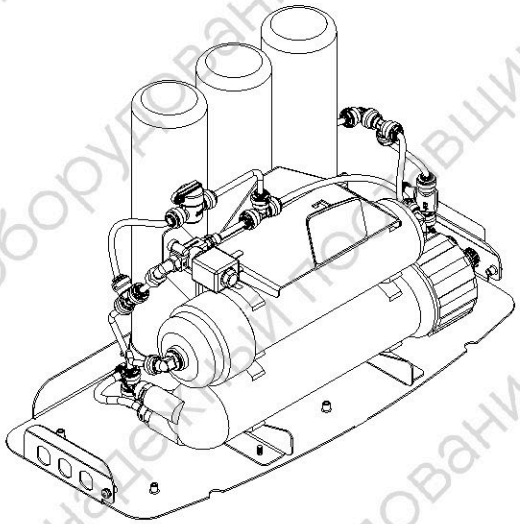

L) When rinsing is complete, close the tap on the solenoid valve.

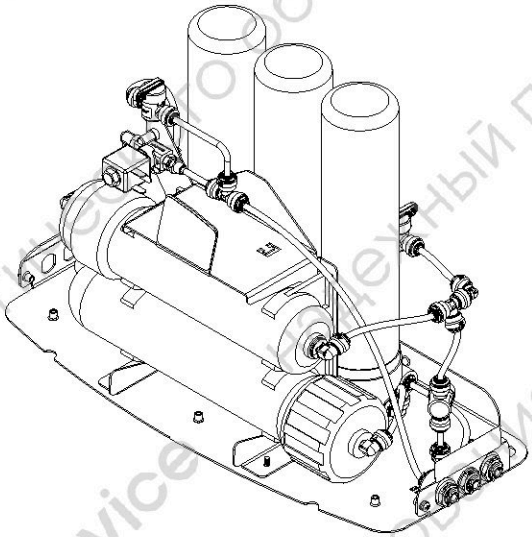


M) Close the drain and open the outlet.

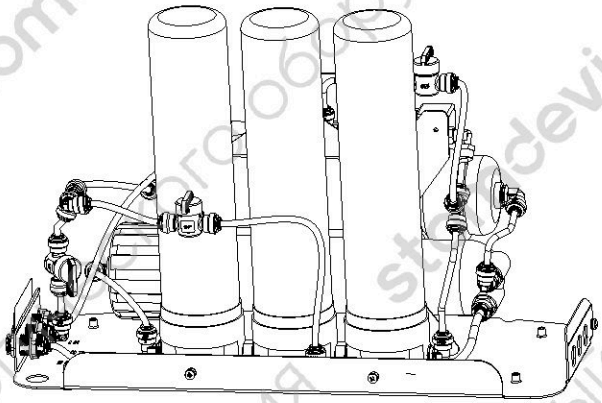

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

N) Reposition the plastic cover on the frame of the demineralizer and secure it with the screws previously removed in point (C).

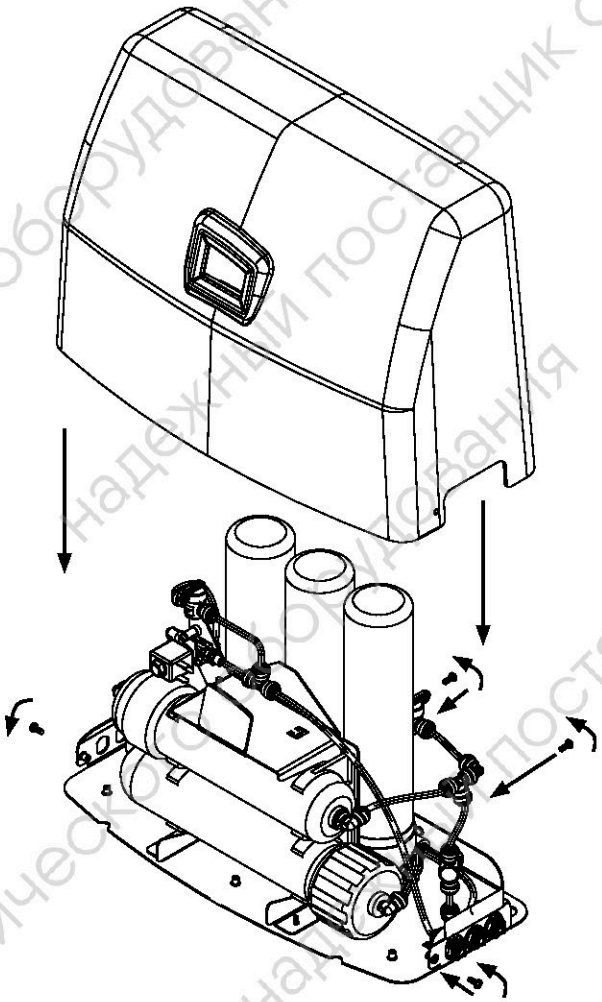


O) Turn on the sterilizer.

P) Wait for automatic filling of the demineralized water tank of the sterilizer.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

APPENDIX C - MANTEINANCE

WATER BLOCK® SAFETY VALVE MAINTENANCE



It is recommended to clean the filter at the inlet to the WATER BLOCK® valve periodically. Carefully follow the instructions in the instruction leaflet contained in the relative package.

PERIODIC CHECK OF THE ANTI-BACKFLOW DEVICES

WARNING!

IN COMPLIANCE WITH THE EN1717 STANDARDS, THE WATER BLOCK® SAFETY VALVE AND THE NON-RETURN VALVE MUST BE CHECKED AT LEAST ONCE A YEAR, PREFERABLY AT THE SAME TIME TECHNICAL SERVICE CARRIES OUT THE MAINTENANCE OPERATIONS ON THE STERILIZER.

DISPOSAL AT END-OF-LIFE

In accordance with Directive 2012/19/UE, regarding the reduction in use of dangerous substances in electrical and electronic equipment, as well as waste disposal, such equipment may not be disposed of as normal urban waste and must be separated accordingly. When purchasing a new, equivalent piece of equipment, the old piece of equipment that has reached its end-of-life must be handed over to the reseller for proper disposal. The Manufacturer will carry out the functions defined by individual national legislation with respect to the reuse, recycling and other forms of salvaging of the above-mentioned waste. The proper collection and separation of such equipment for recycling, treatment and disposal helps avoid any possible negative effects on the environment and health and facilitates the recycling of the materials of which the equipment is made. The crossed out rubbish can symbol indicates that the product, at the end-of-life, must be collected separately from other types of waste.

WARNING!

IMPROPER DISPOSAL OF THE PRODUCT RESULTS IN THE APPLICATION OF SANCTIONS WHICH ARE DEFINED BY INDIVIDUAL NATIONAL LAWS.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

APPENDIX D - TROUBLESHOOTING

If the demineralizer does not function properly, carry out the following checks before calling Technical Service:

WARNING	POSSIBLE CAUSE	ACTION
The message “H2O quality insufficient” is shown on the autoclave display.	-The demineralizer is working but is producing demineralized water with conductivity values higher than permitted (resin cartridges exhausted).	-Replace the ionic exchange resin cartridges.

NOTE

IF THE PROBLEM PERSISTS, CONTACT THE TECHNICAL SUPPORT SERVICE (SEE APPENDIX Z) REPORTING THE THERMO-SEALER MODEL AND ITS SERIAL NUMBER.

THESE DATA CAN BE FOUND ON THE FACTORY PLATE PLACES ON THE UNIT REAR.

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ

stomdevice

APPENDIX Z - CUSTOMER SUPPORT

FOR ANY REQUEST FOR TECHNICAL SERVICE FOR THE PRODUCT,WHETHER IN OR OUT OF WARRANTY, DIRECTLY CONTACT THE TECHNICAL SUPPORT DEPARTMENT OF THE DEALER OR RESELLER THAT SUPPLIED THE PRODUCT.

CEFLA S.C. will gladly provide any information you may need on the product as well as give you sugge-stions and advice on the steam sterilization procedures.
In this regard, please refer to the following address:

CEFLA s.c.

Plant
Via Bicocca, 14/C 40026 - Imola (BO) IT
Tel. +39 0542 653441 Fax. +39 0542 653555

Headquarter
Via Selice Provinciale 23/A – 40026 Imola (BO) IT

https://stomdevice.ru - стоматологическое и зуботехническое оборудование с доставкой по России и СНГ